

FIG. 1

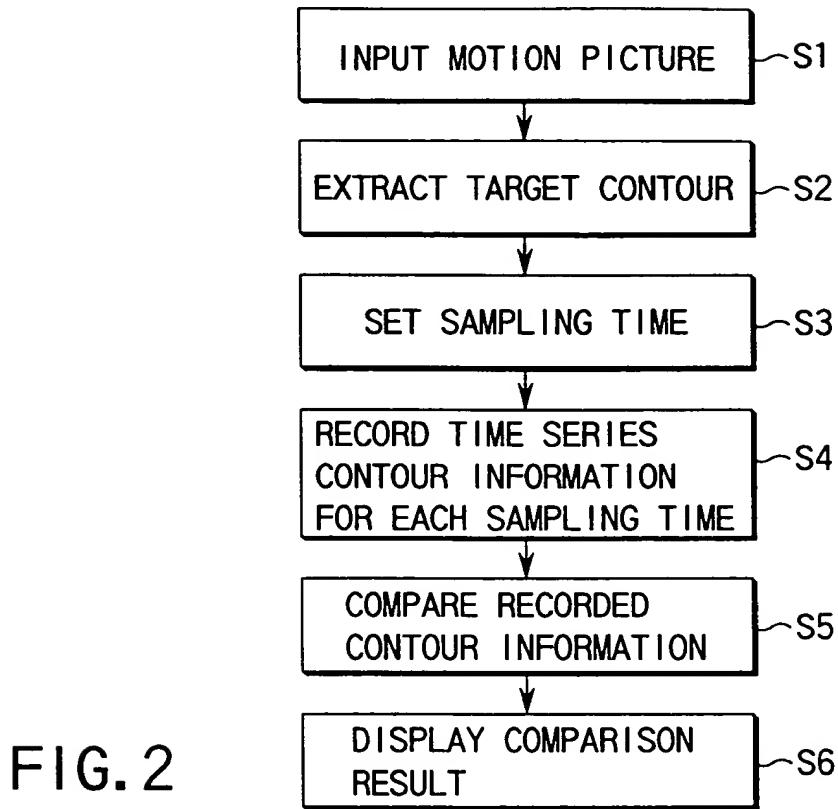


FIG. 2

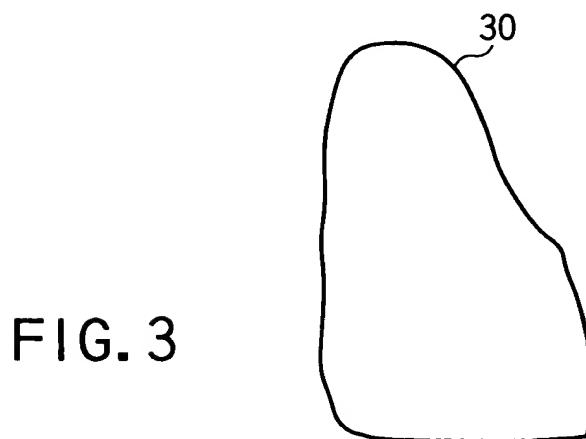


FIG. 3

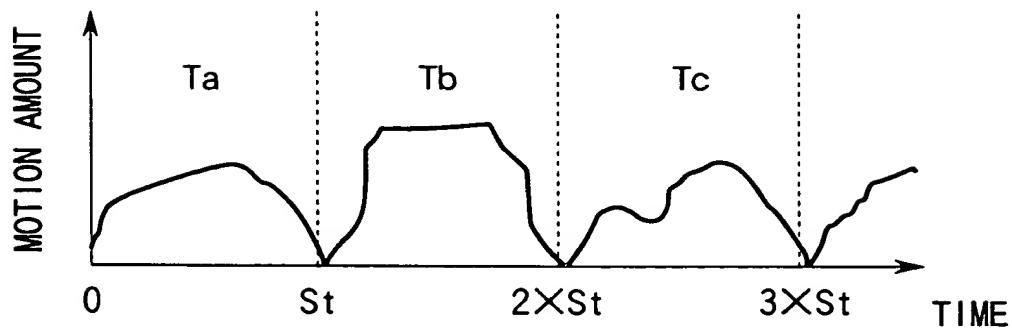


FIG. 4

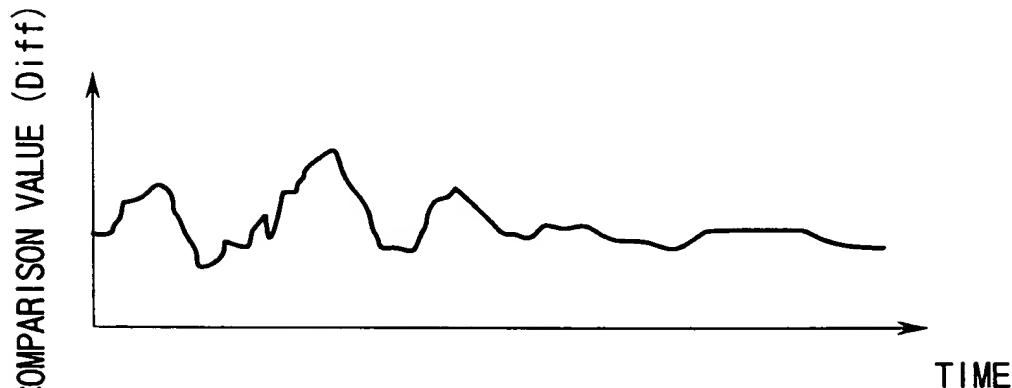


FIG. 5

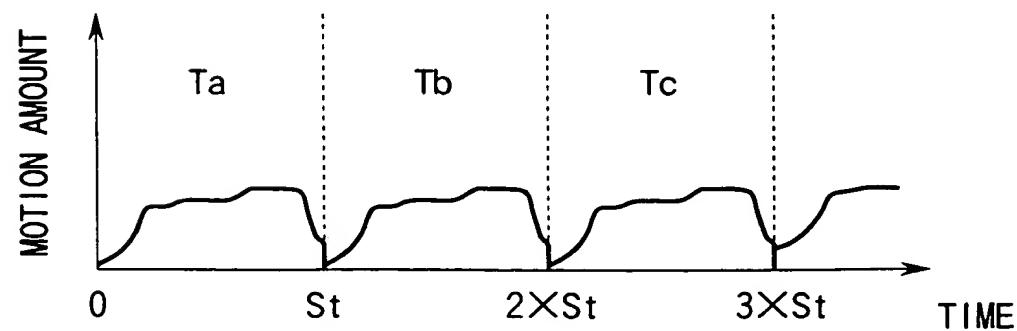
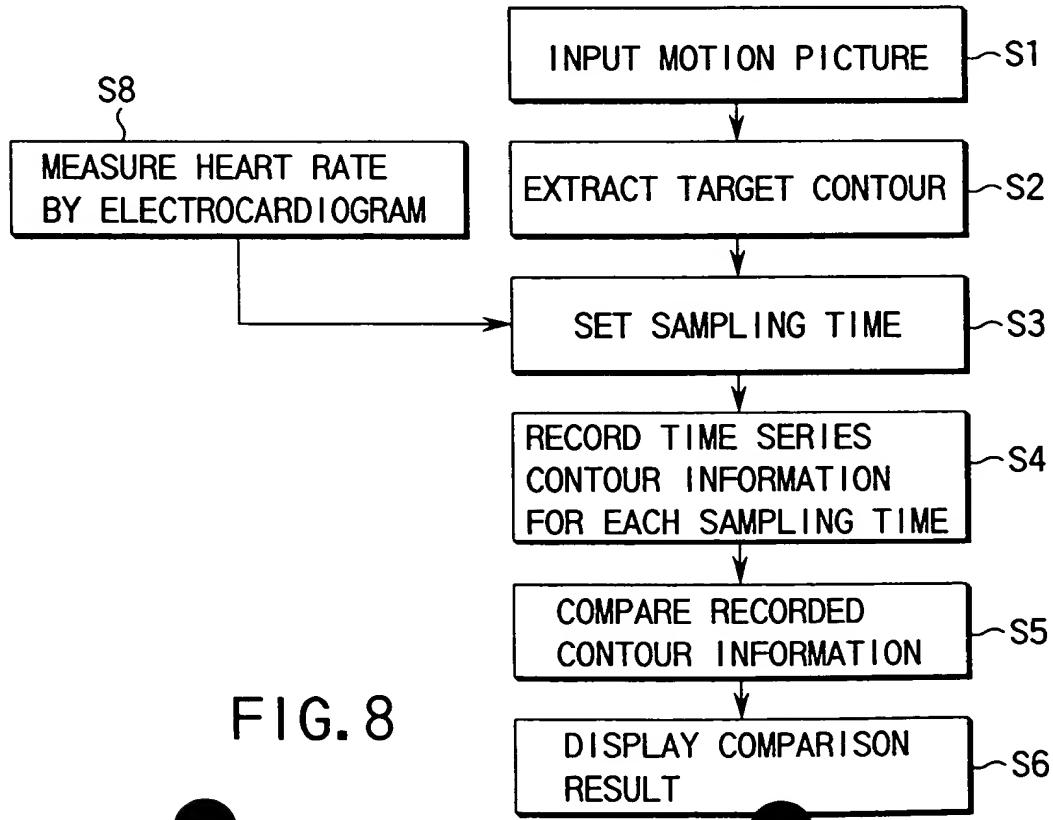
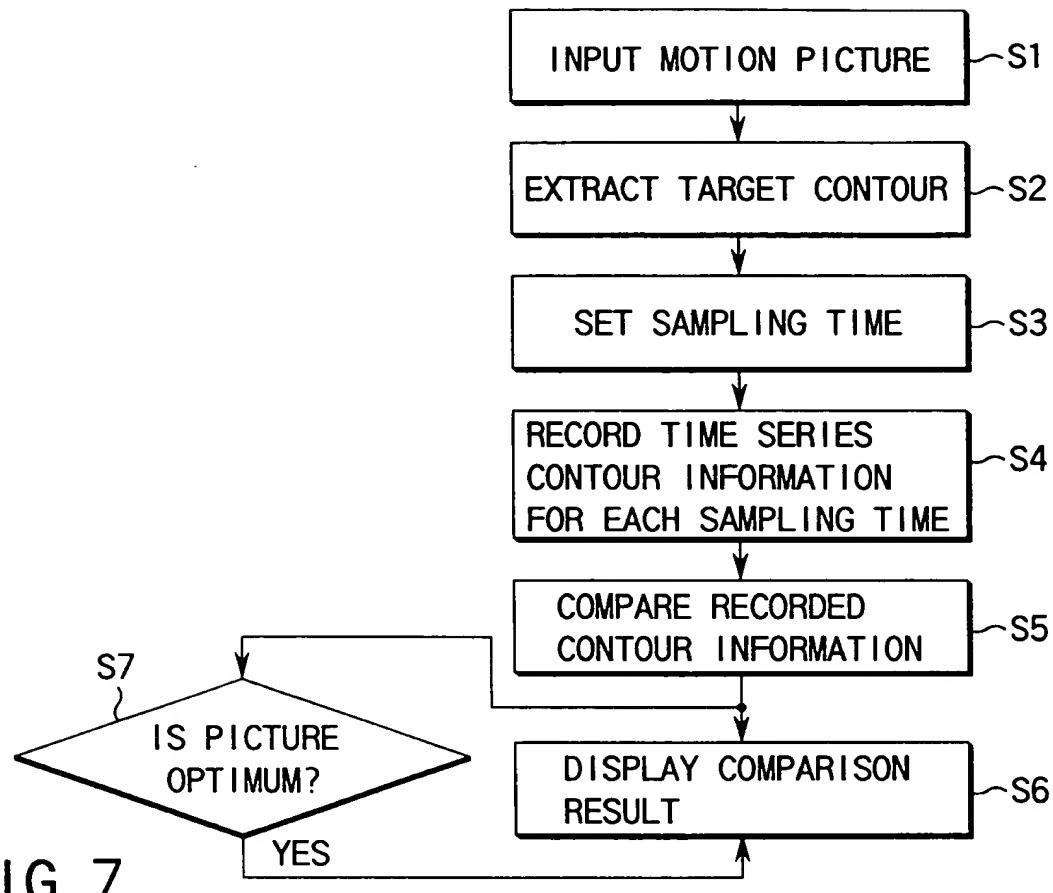


FIG. 6



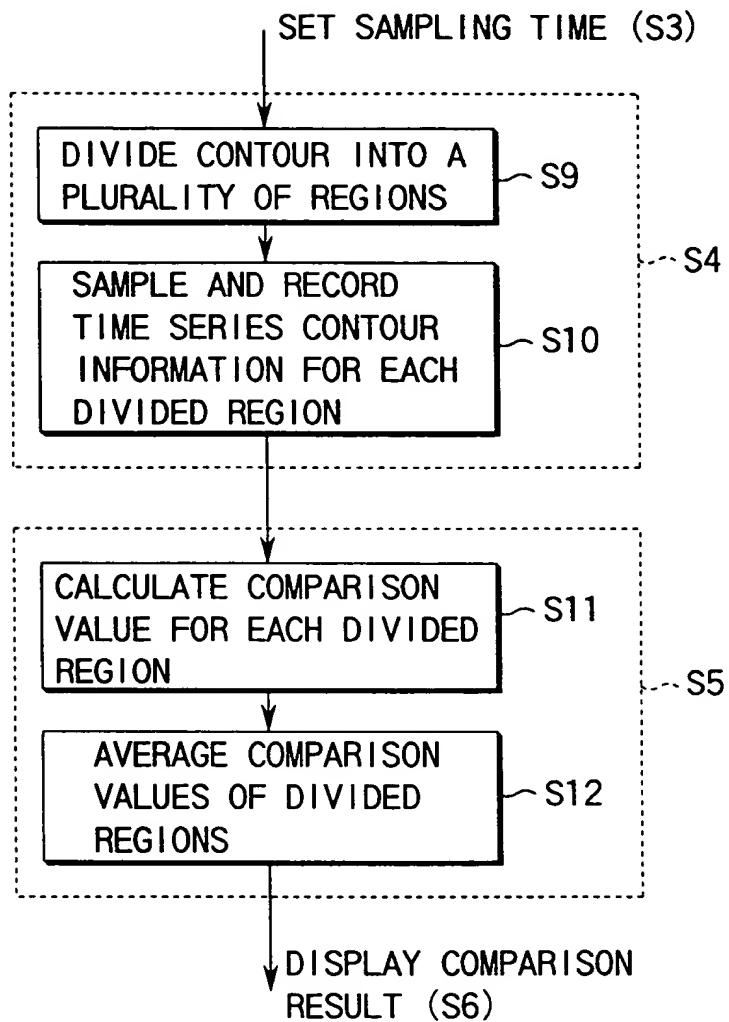


FIG. 9

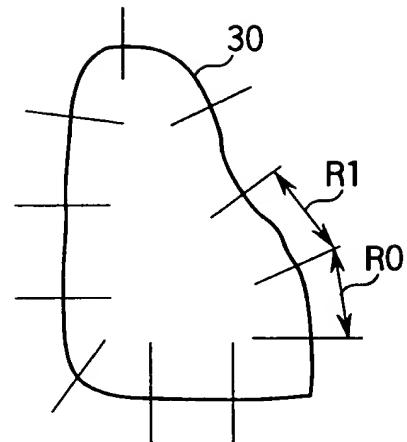


FIG. 10

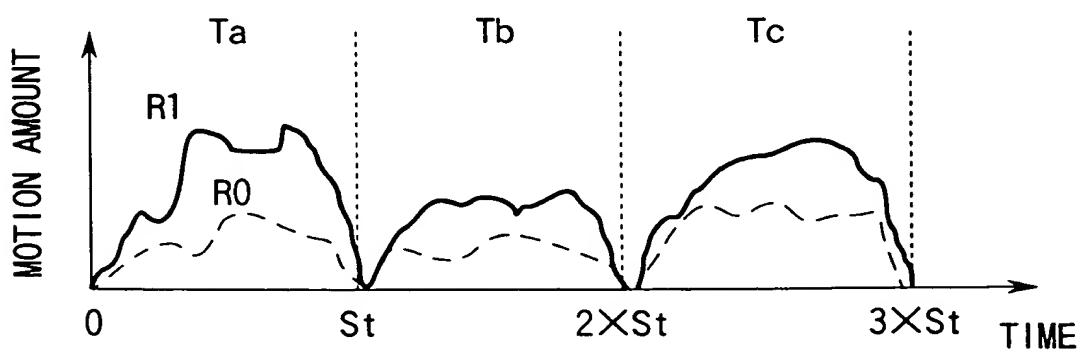


FIG. 11

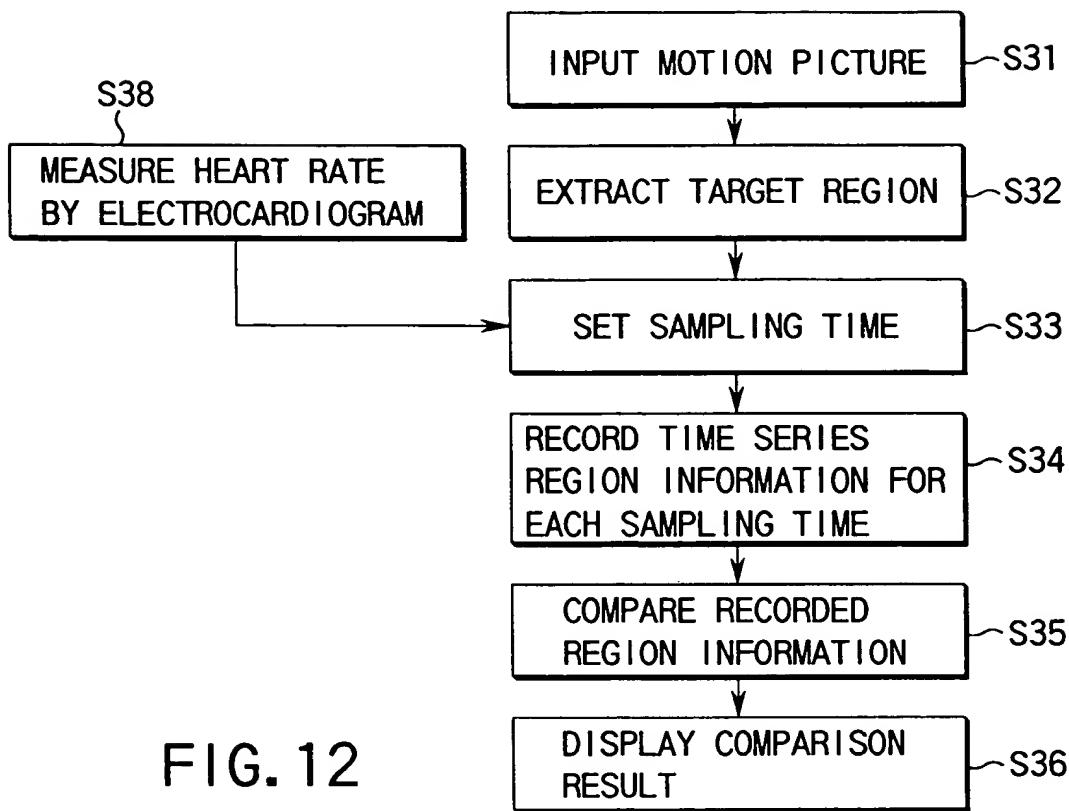


FIG. 12

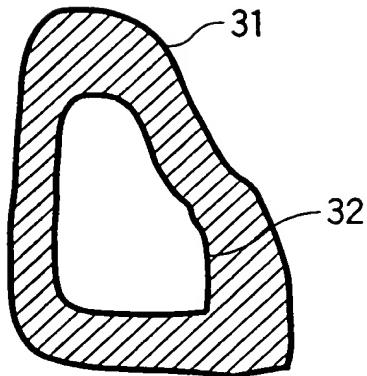


FIG. 13

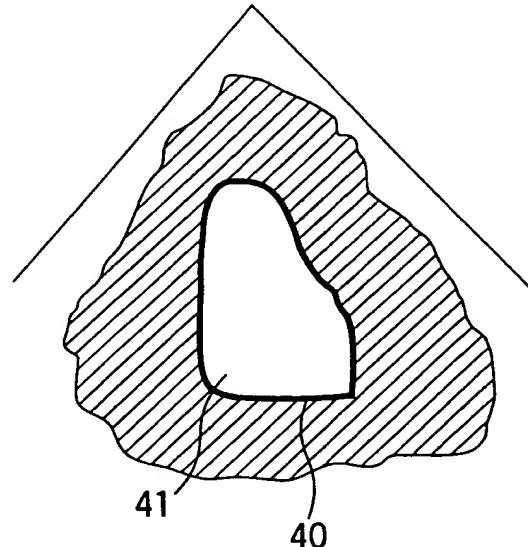


FIG. 14

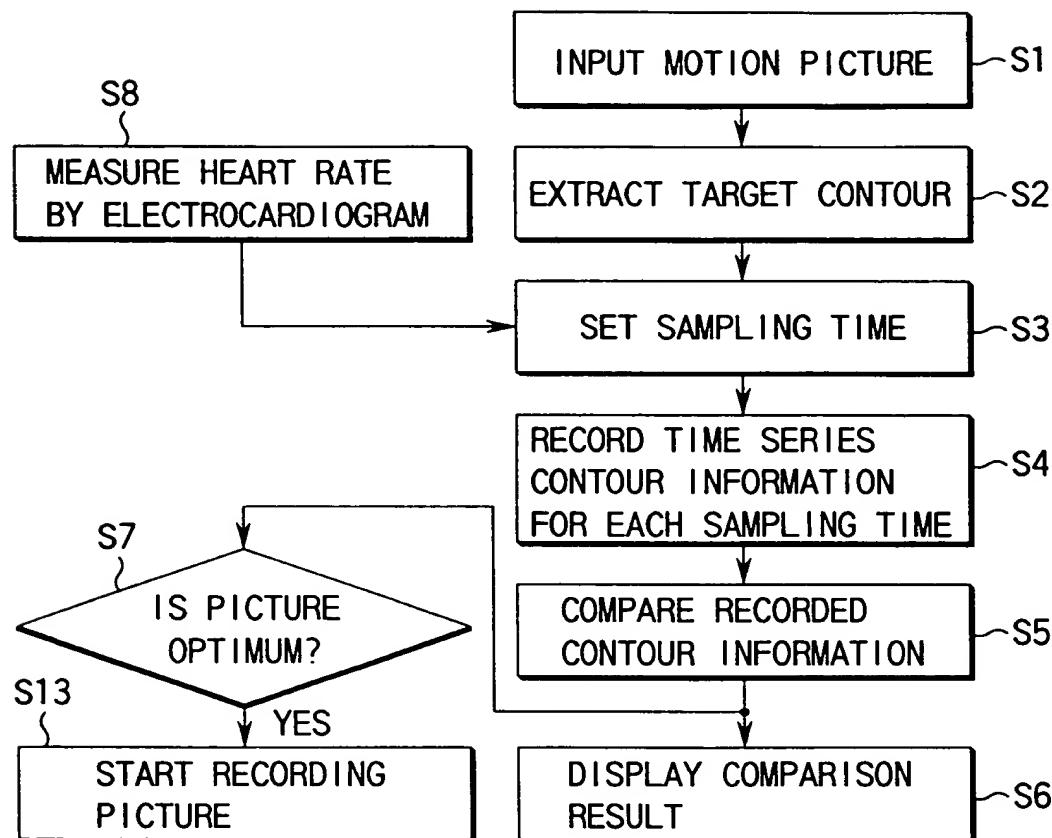


FIG. 15

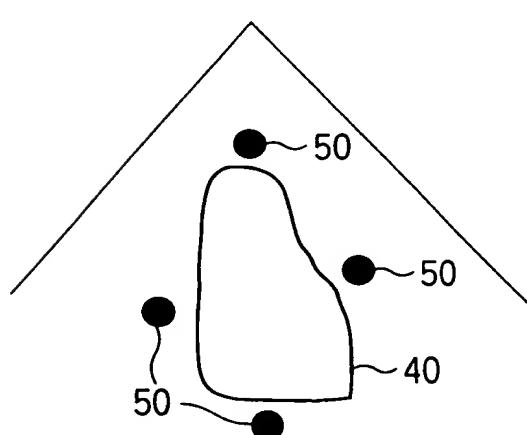


FIG. 16

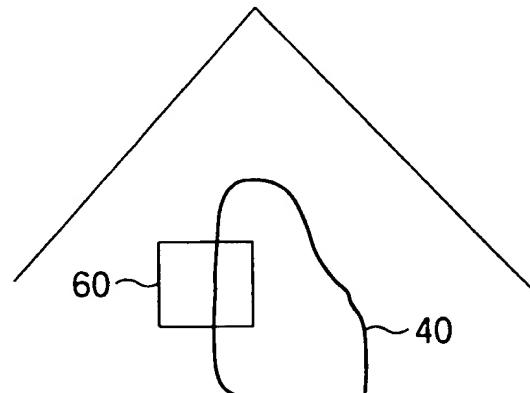


FIG. 17

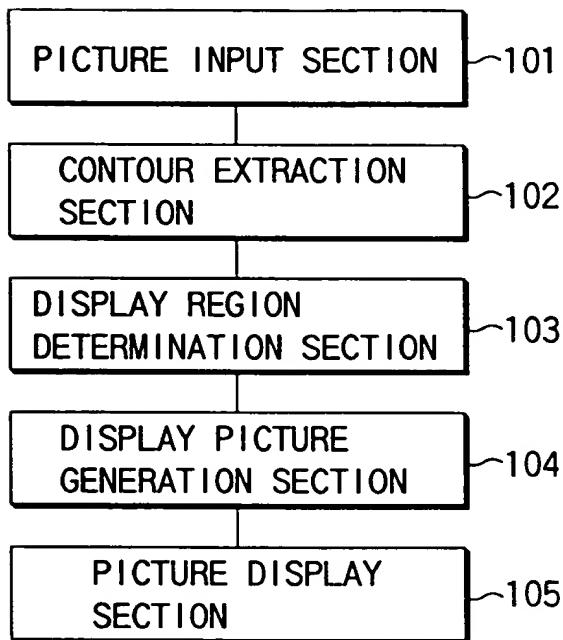


FIG. 18

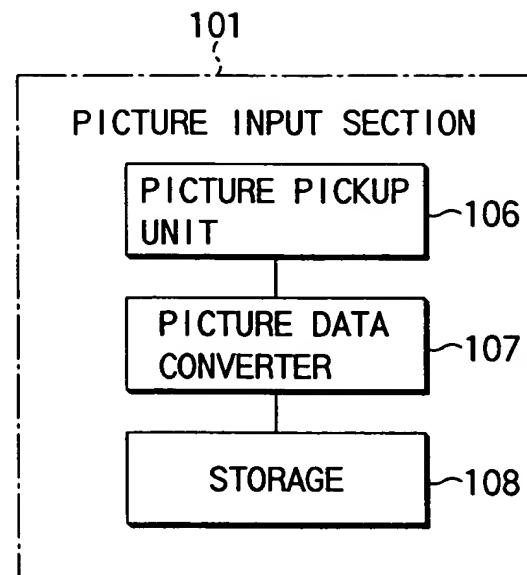


FIG. 19



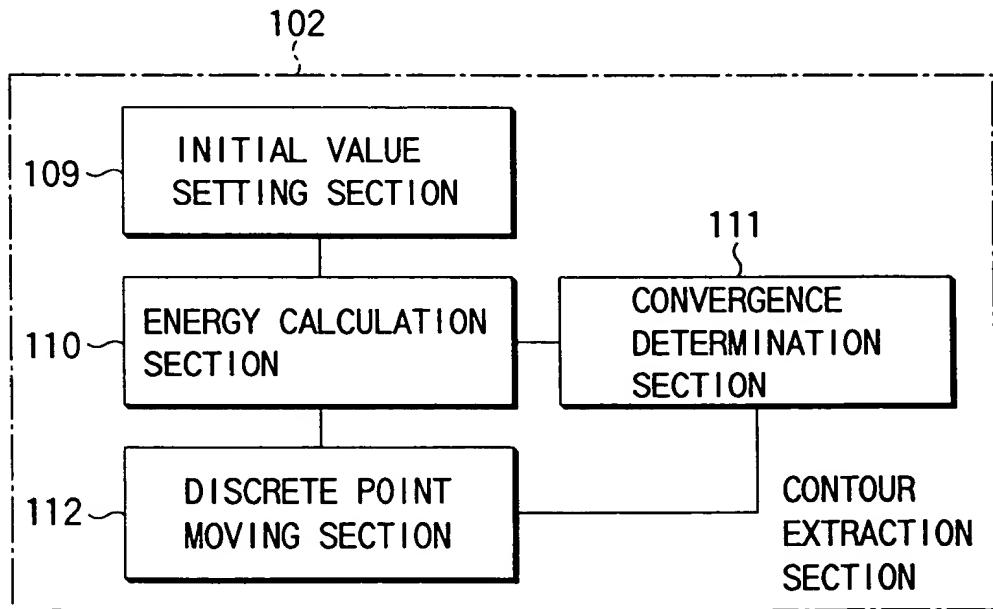


FIG. 20



CONTOUR REGION



DISPLAY REGION

FIG. 21A

FIG. 21B

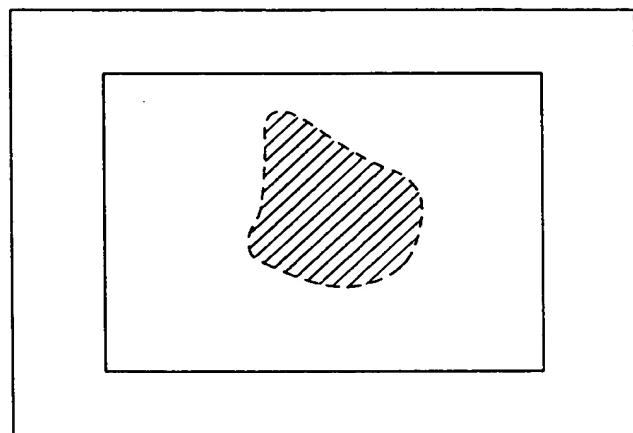


FIG. 22

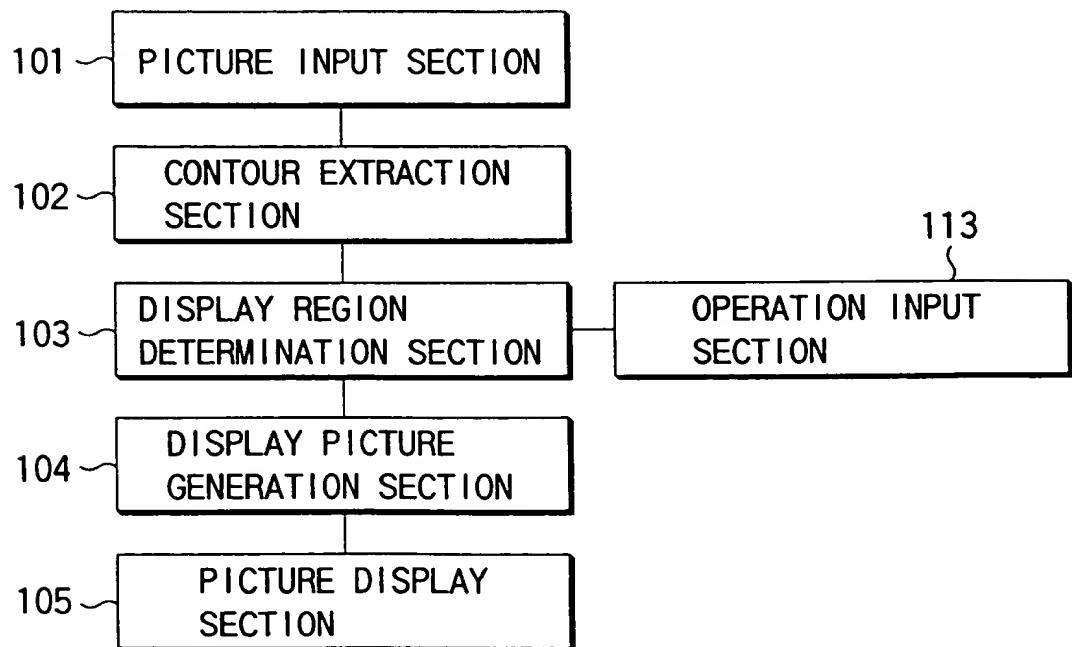


FIG. 23

202907US-2SRD-450

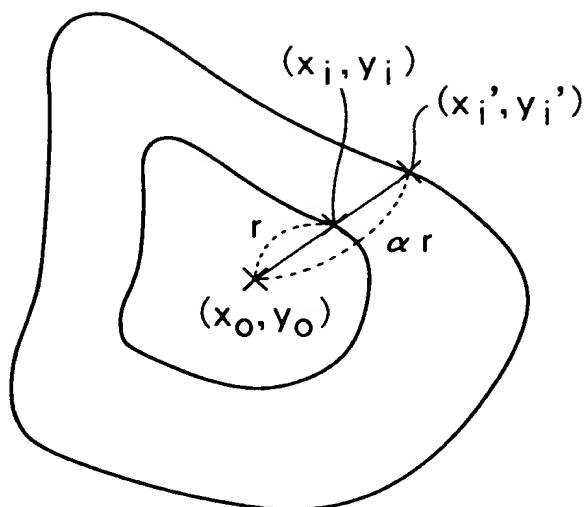


FIG. 24

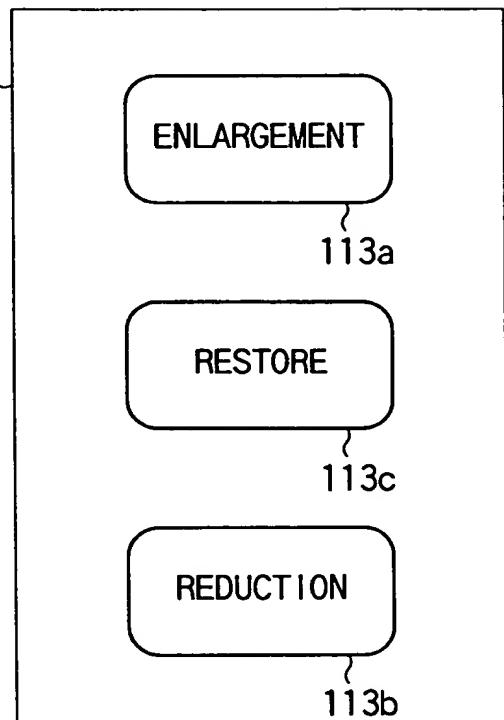


FIG. 25

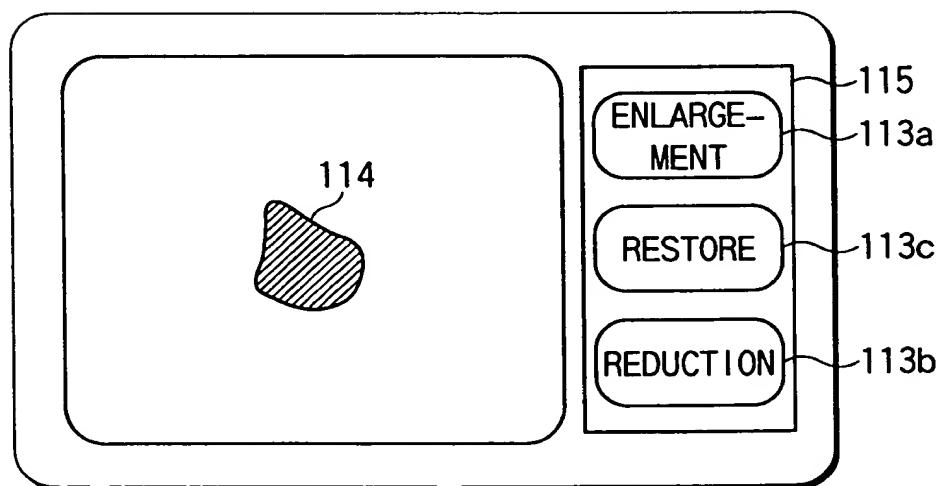


FIG. 26

FIG. 27

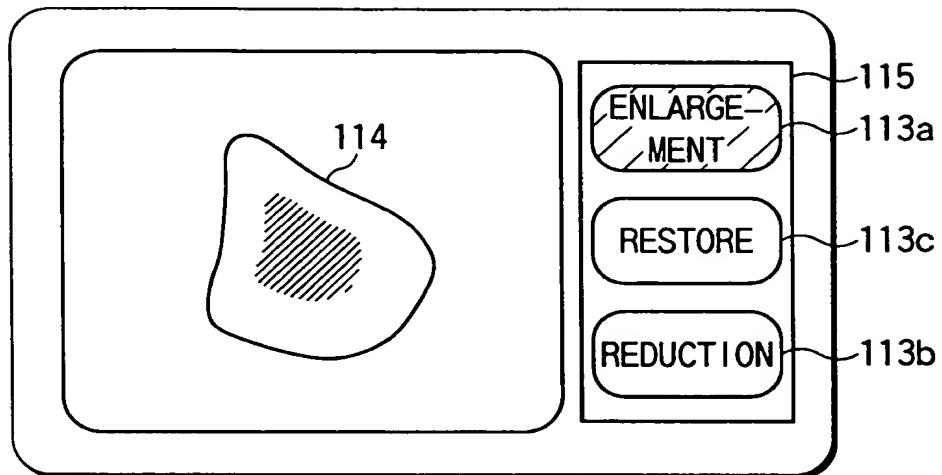


FIG. 28

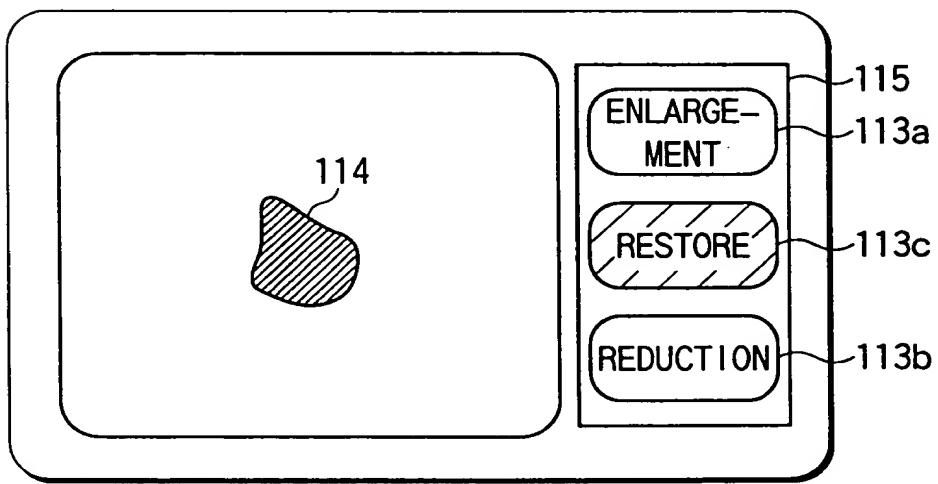


FIG. 29

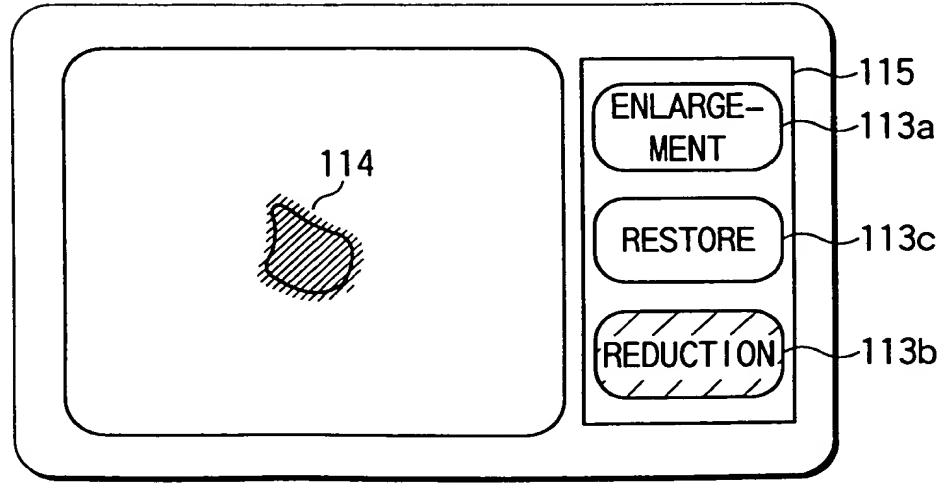


FIG. 30

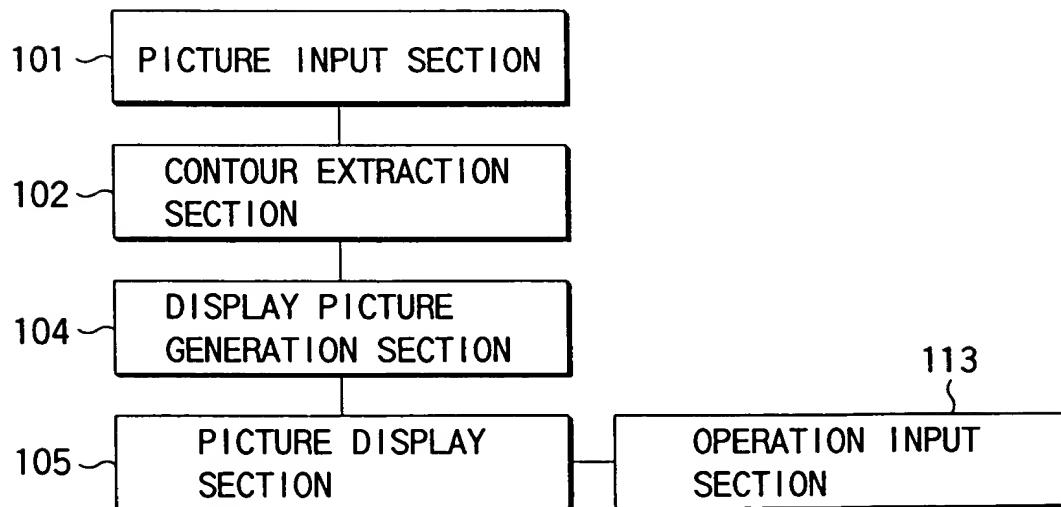
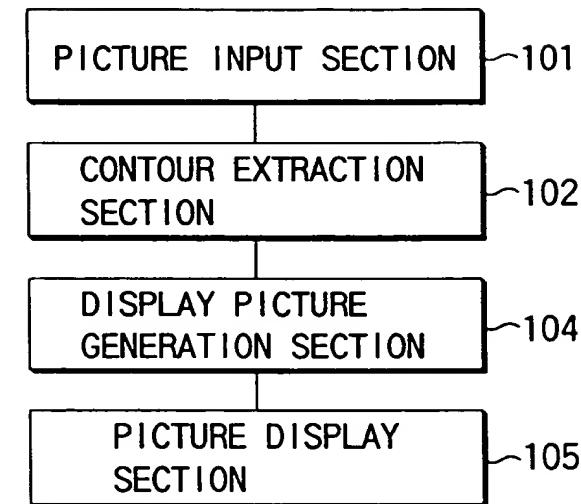


FIG. 31



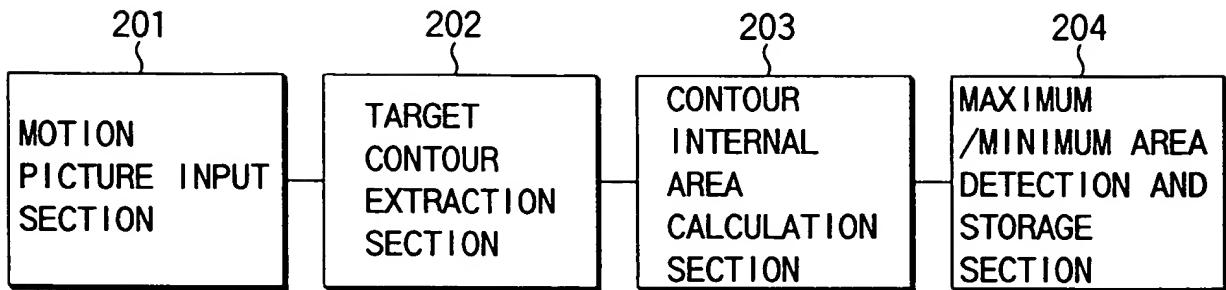


FIG. 32

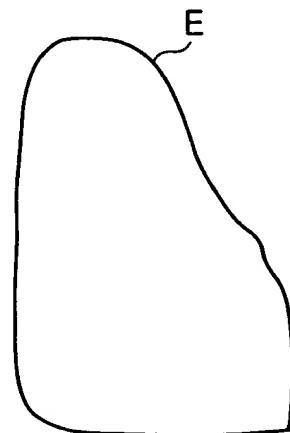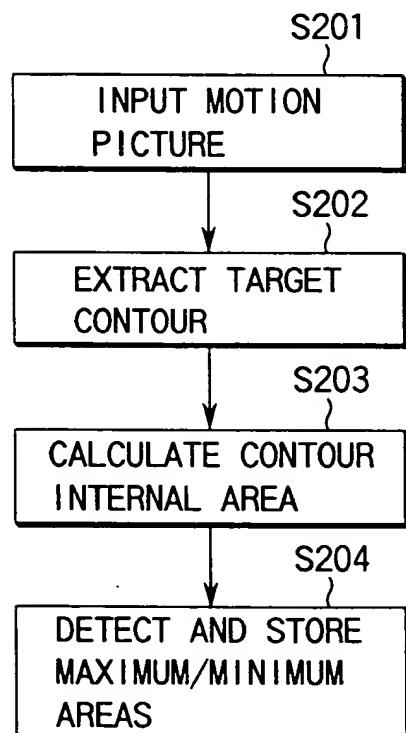

EXTRACTED HEART CONTOUR

FIG. 33

FIG. 34

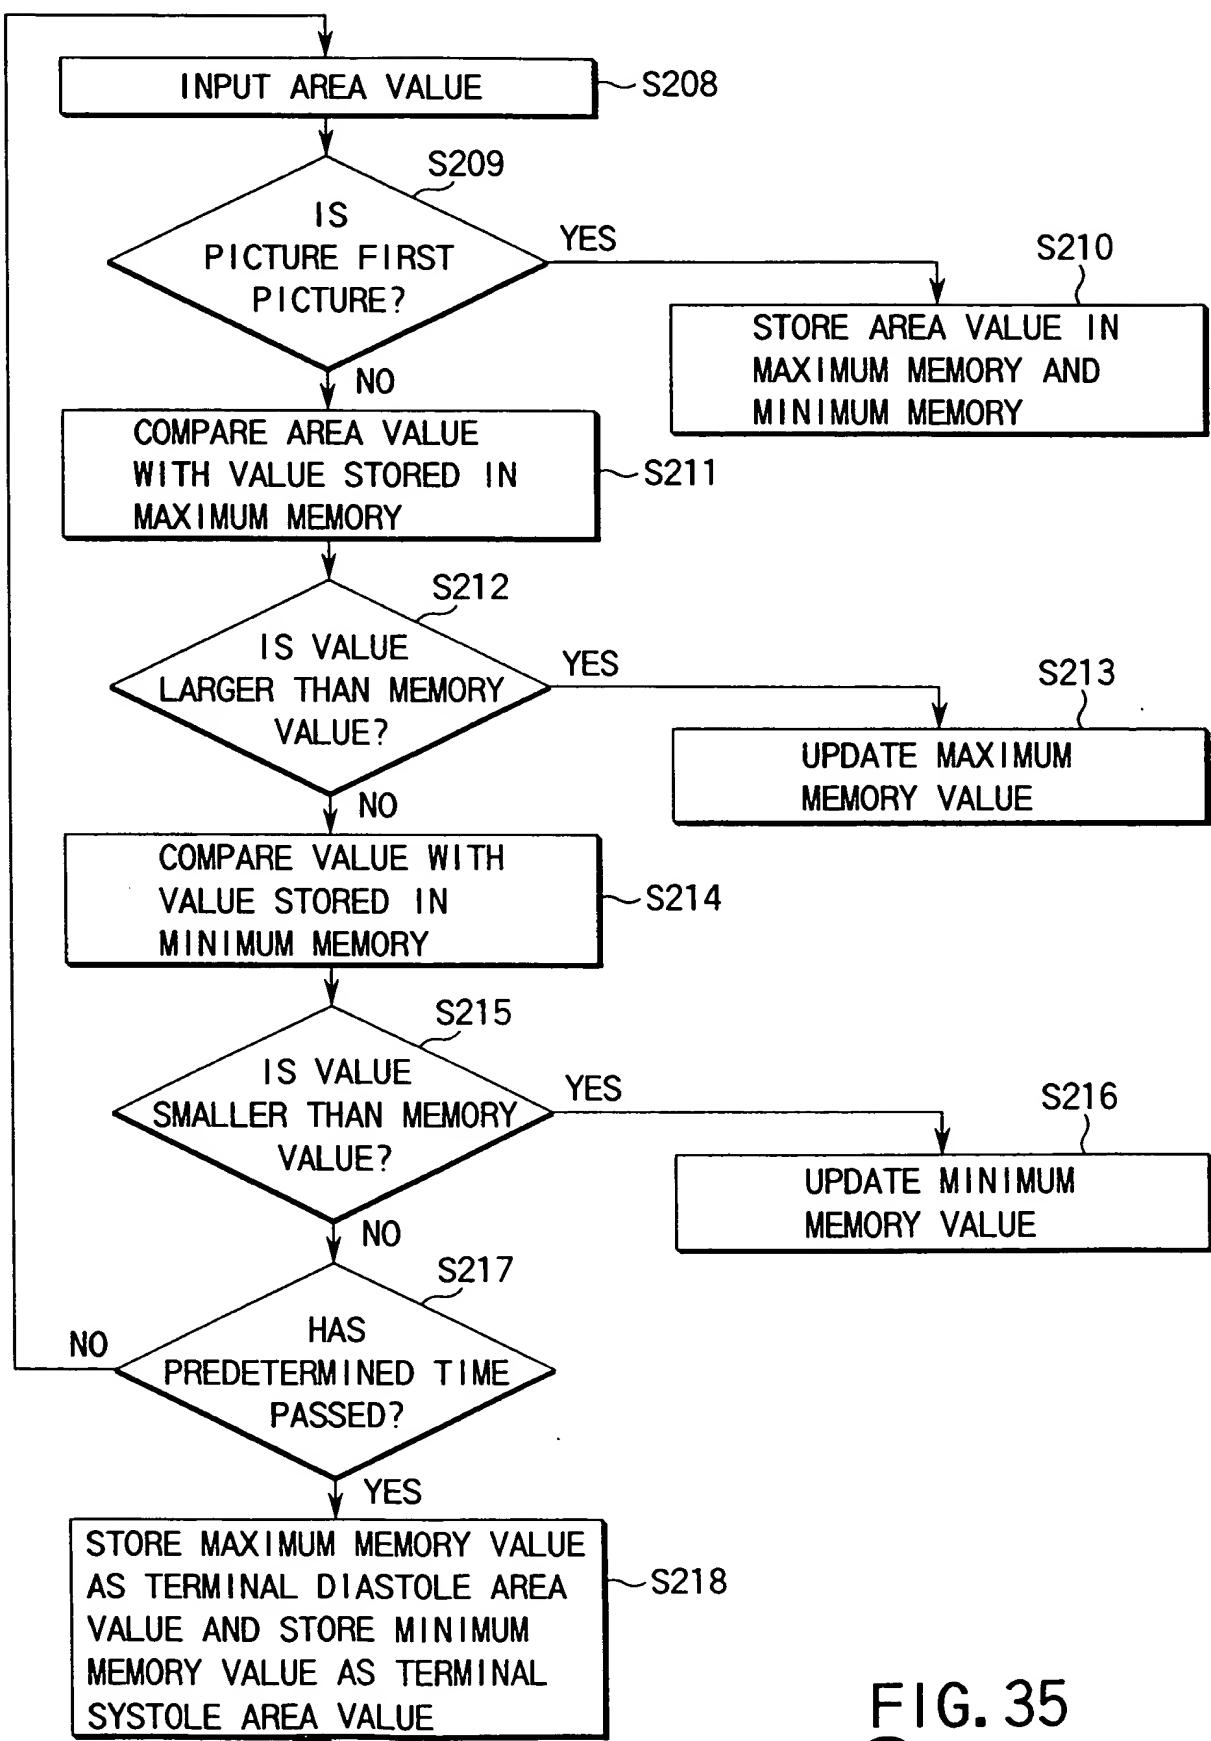


FIG. 35

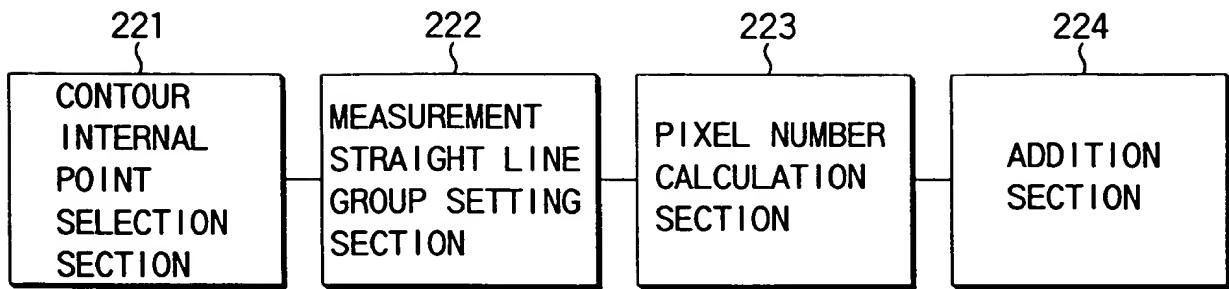


FIG. 36

TO2020-26082260

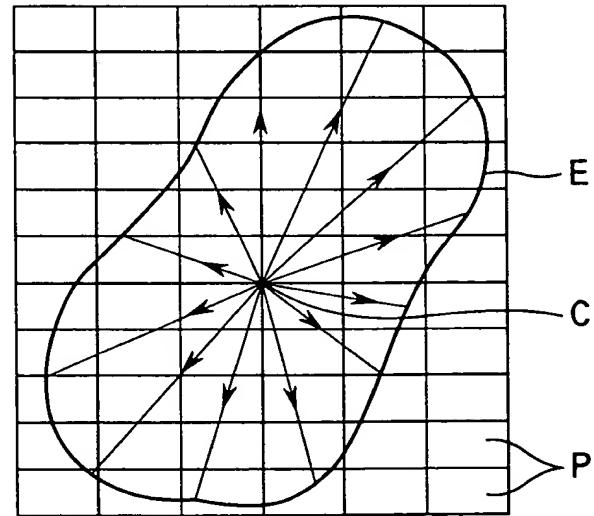
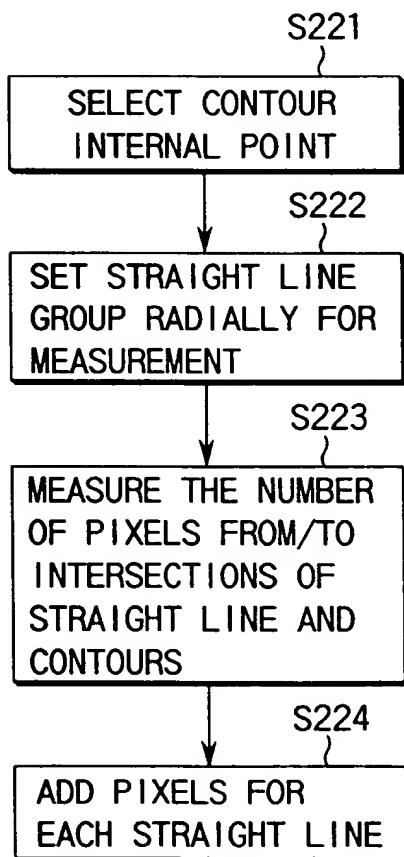


FIG. 38

FIG. 37

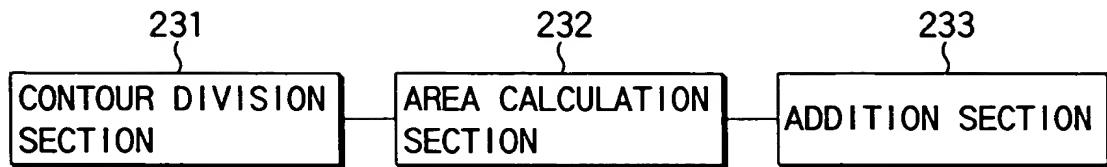


FIG. 39

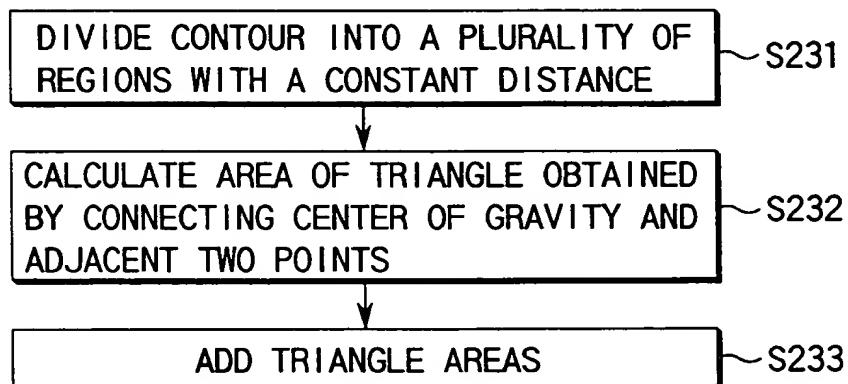


FIG. 40

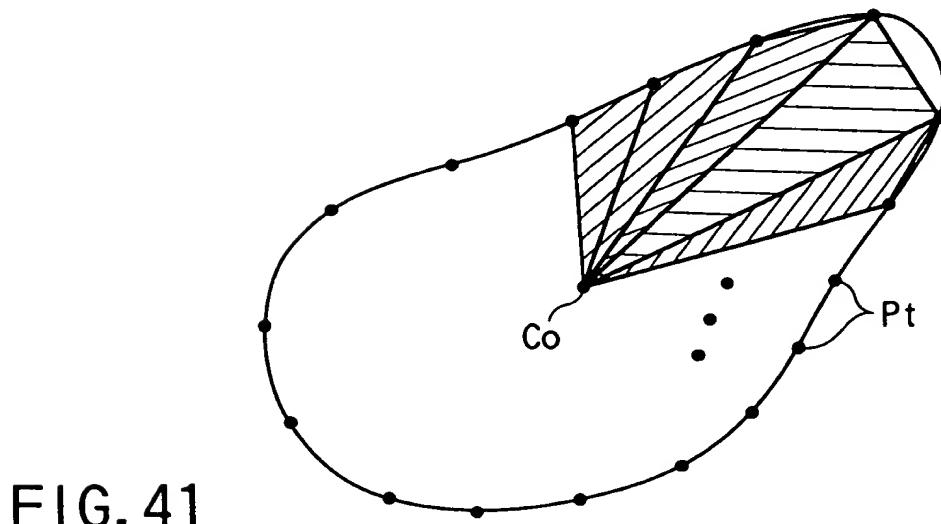


FIG. 41

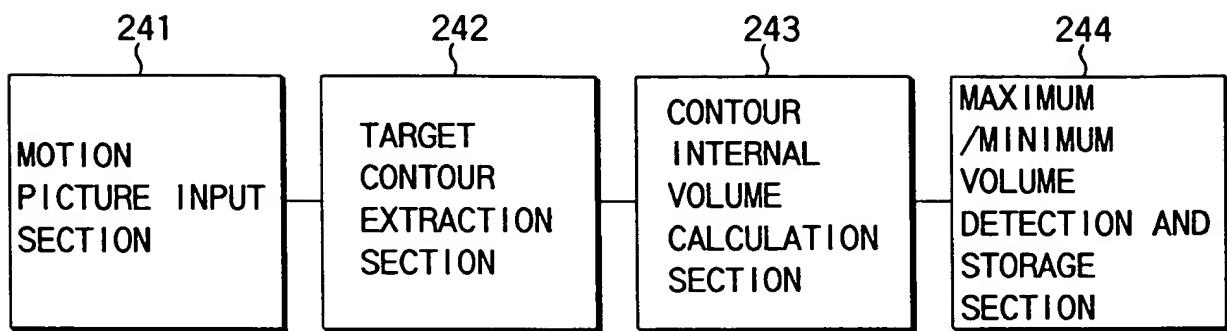


FIG. 42

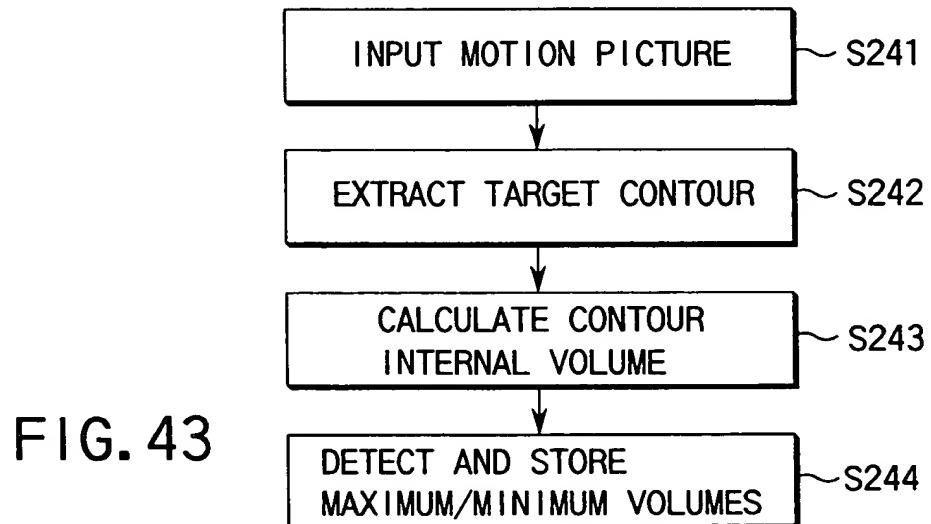


FIG. 43

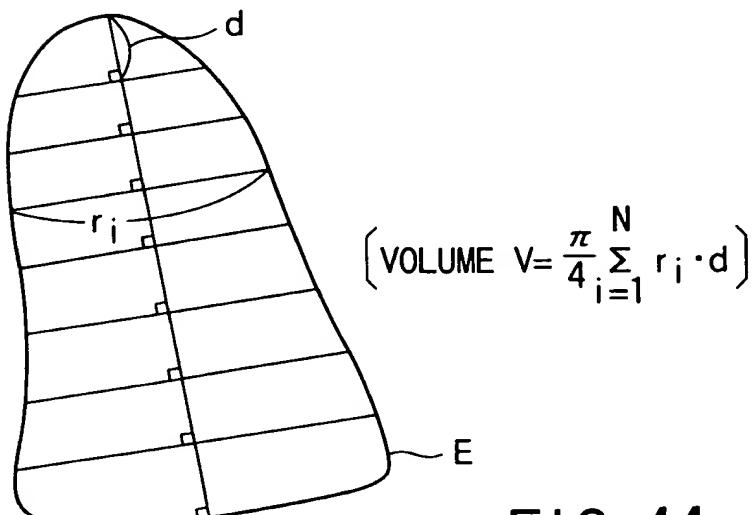


FIG. 44

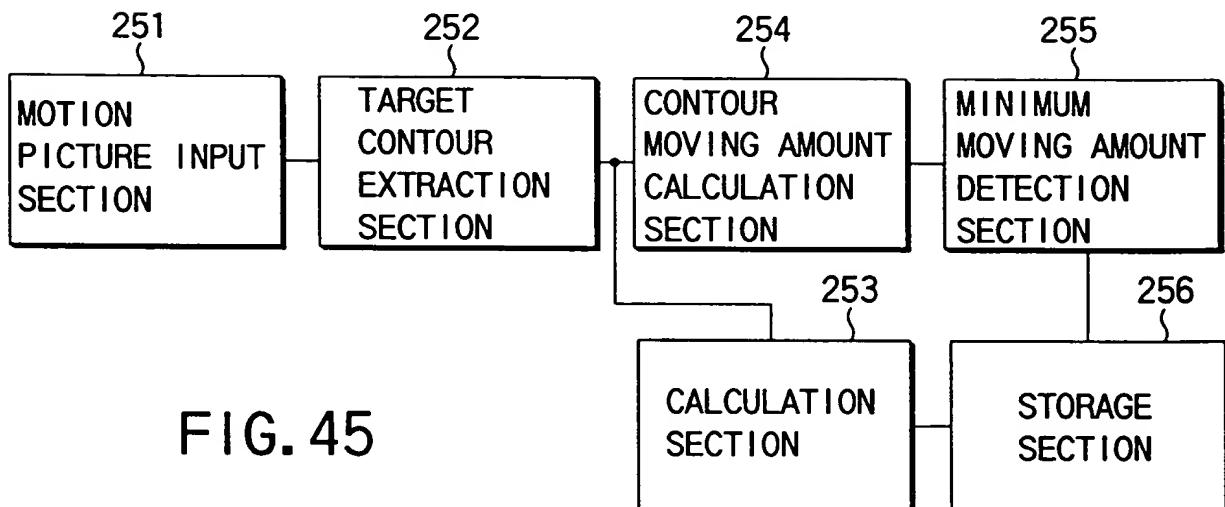


FIG. 45

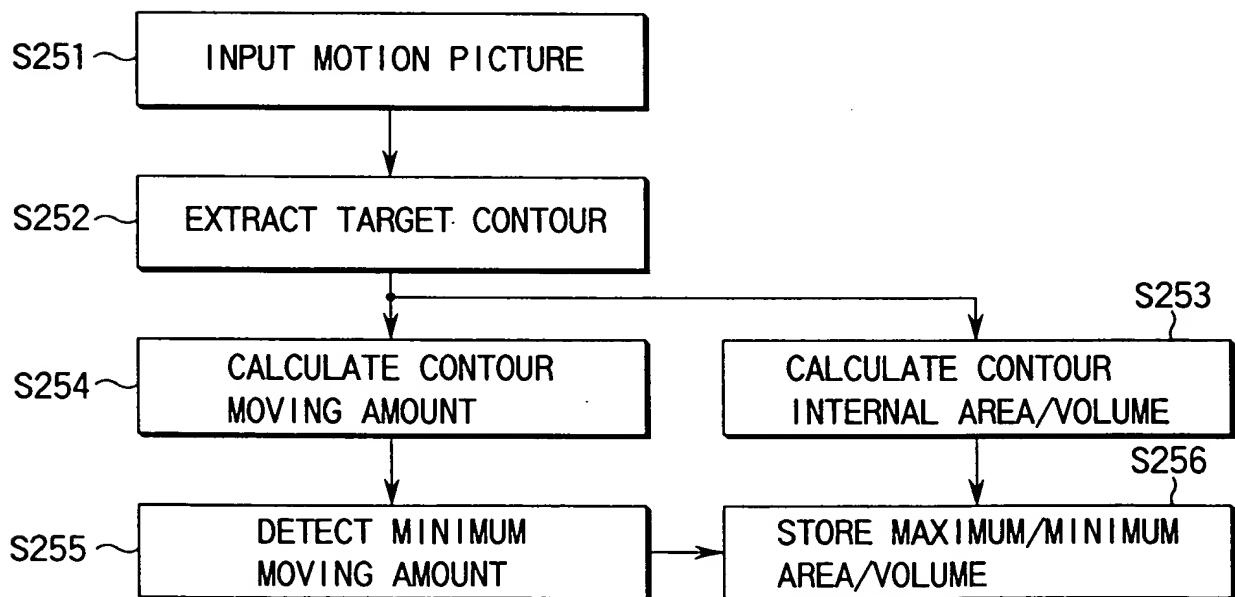


FIG. 46

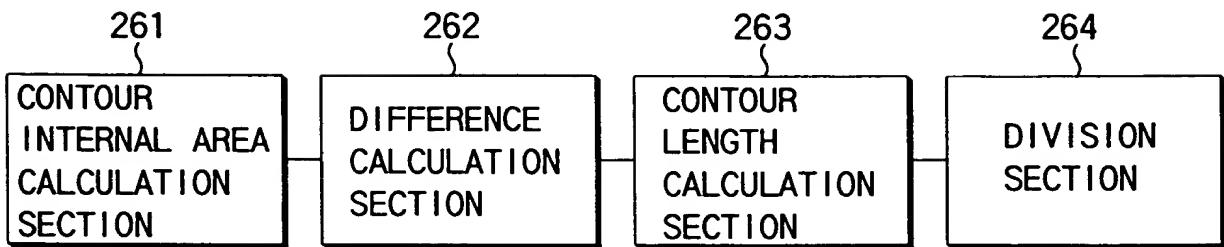


FIG. 47

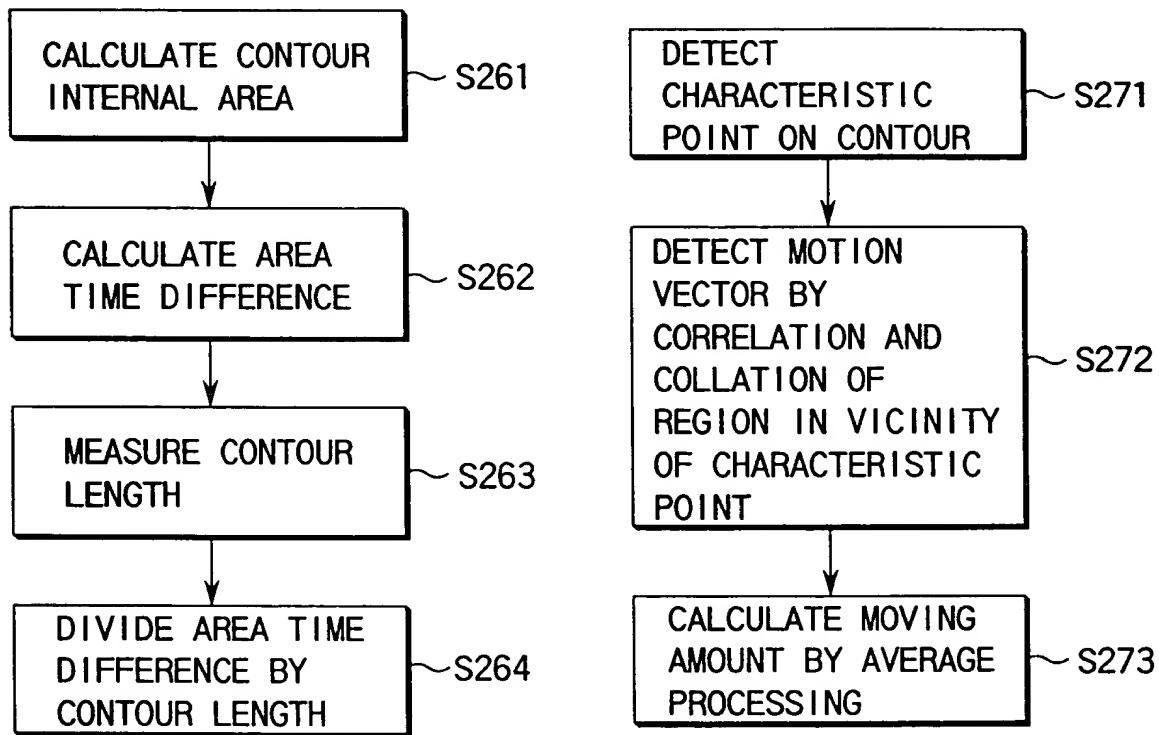


FIG. 48

FIG. 50

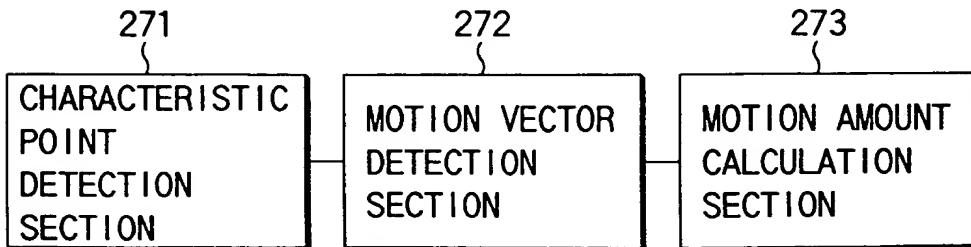


FIG. 49

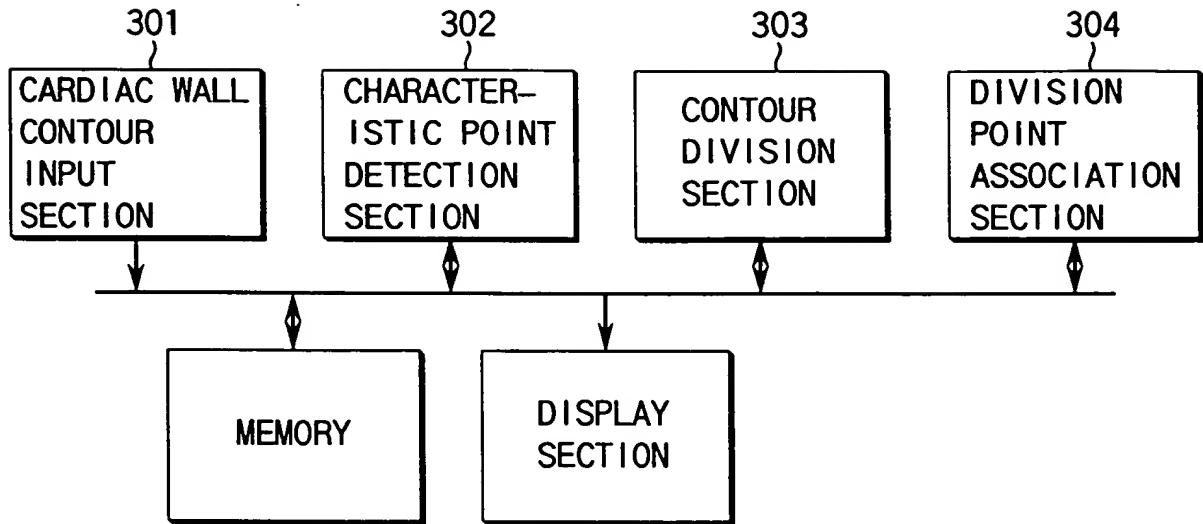


FIG. 51

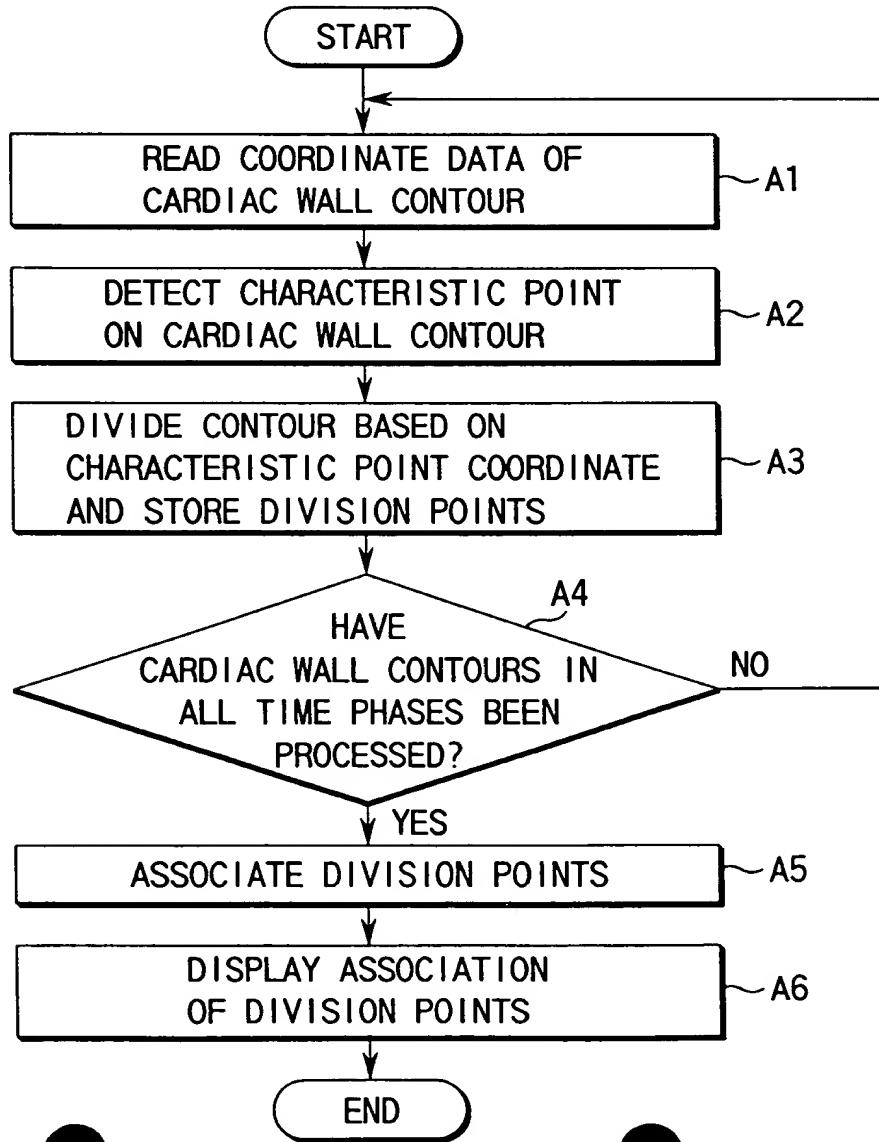


FIG. 52

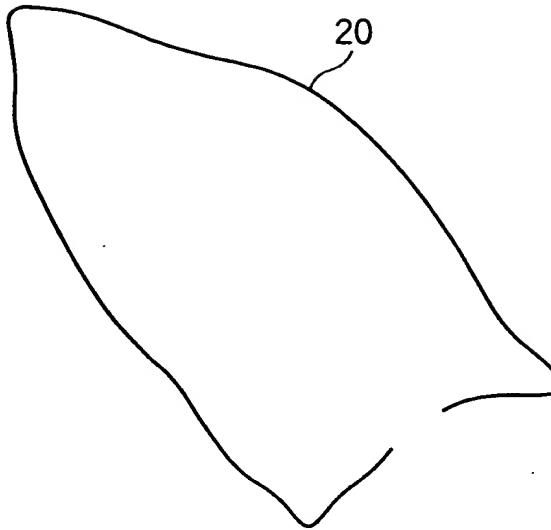


FIG. 53

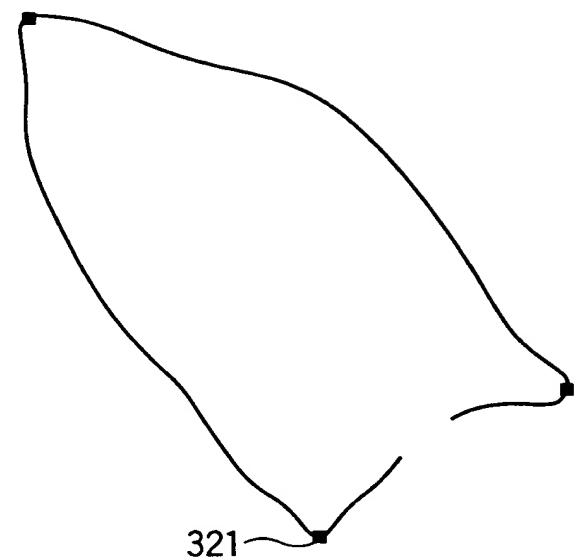


FIG. 54

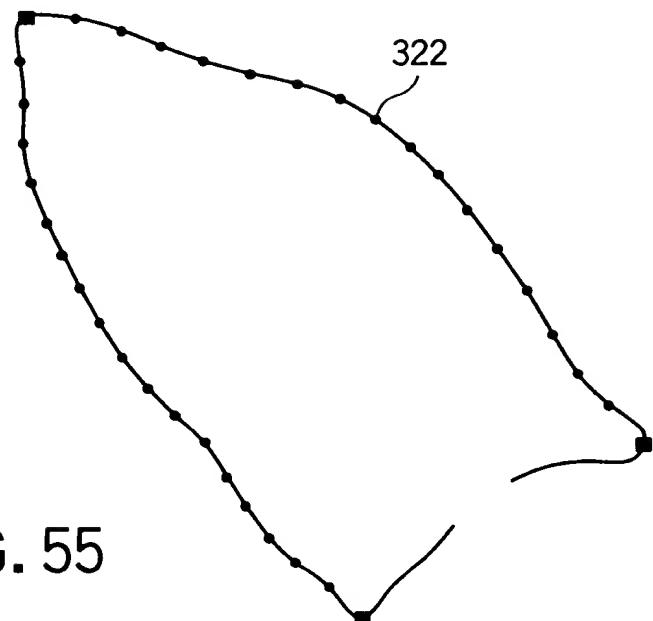
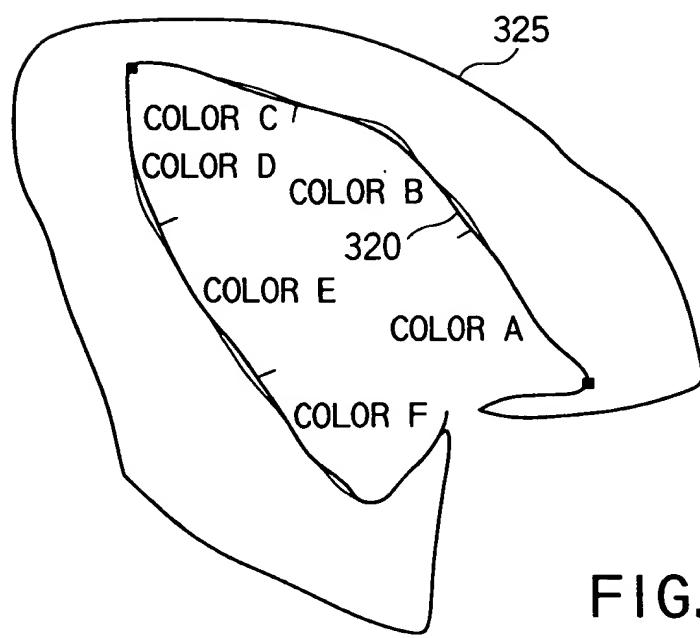
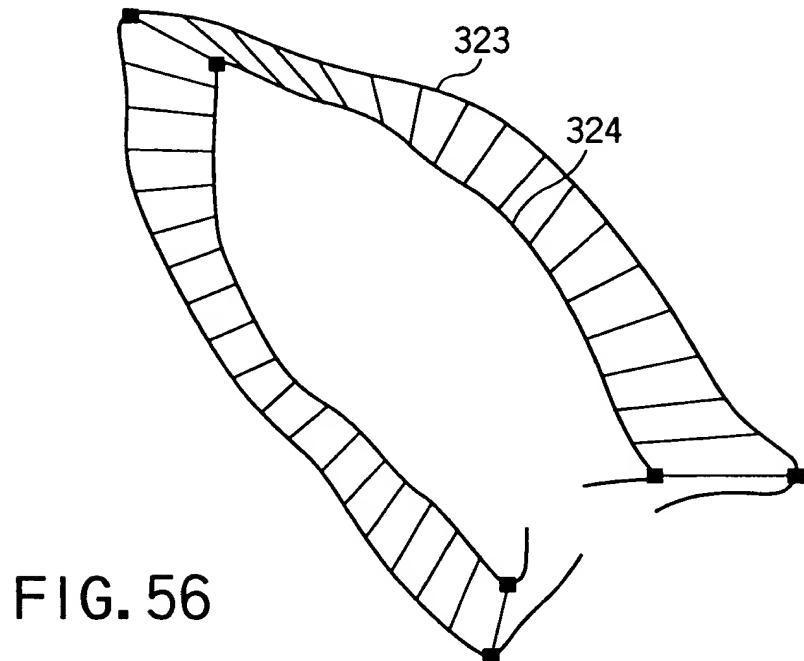


FIG. 55



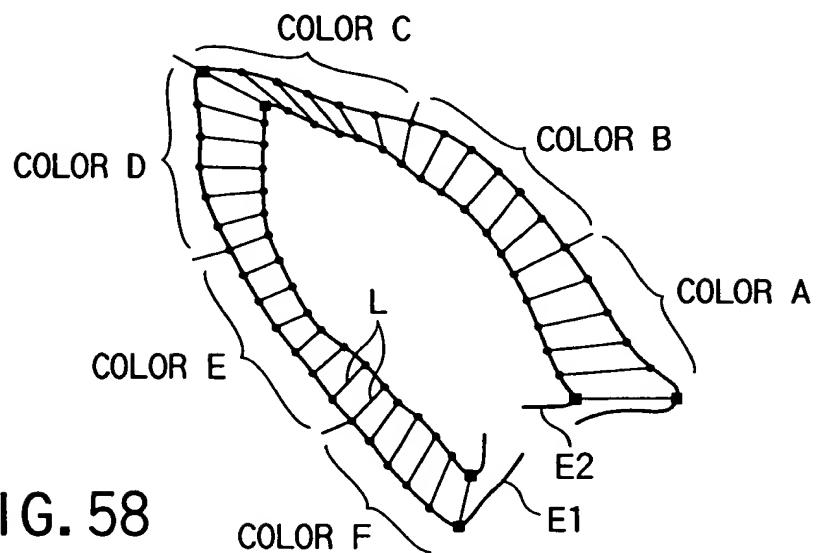


FIG. 58

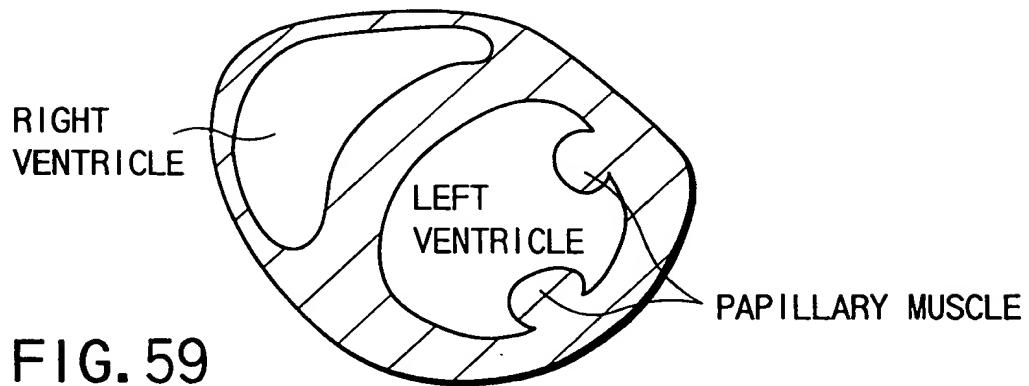


FIG. 59

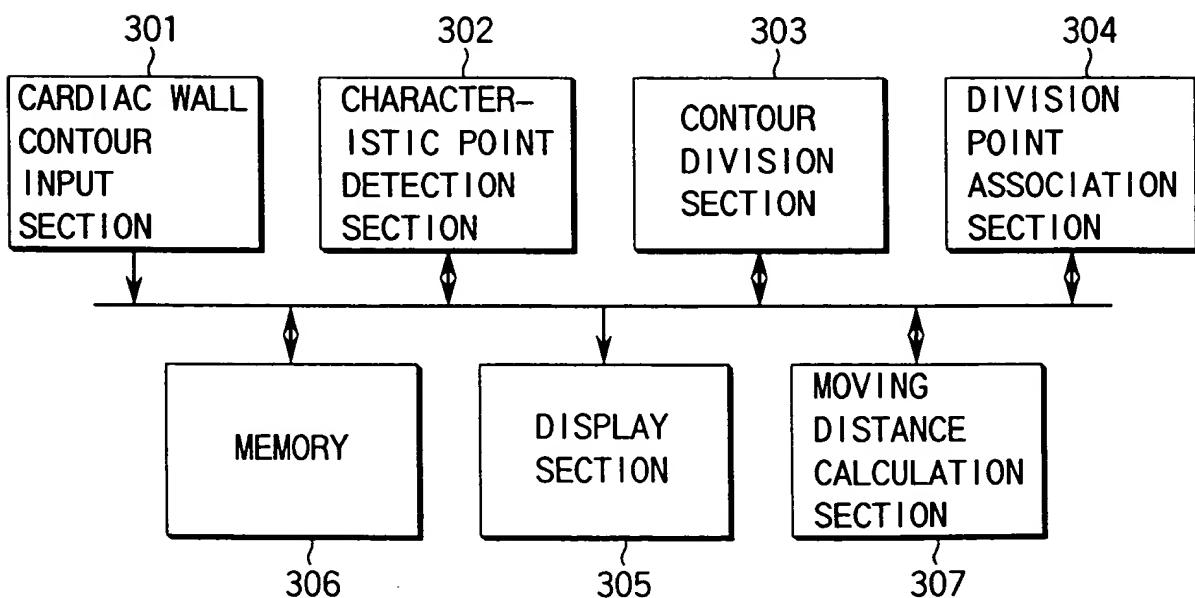


FIG. 60

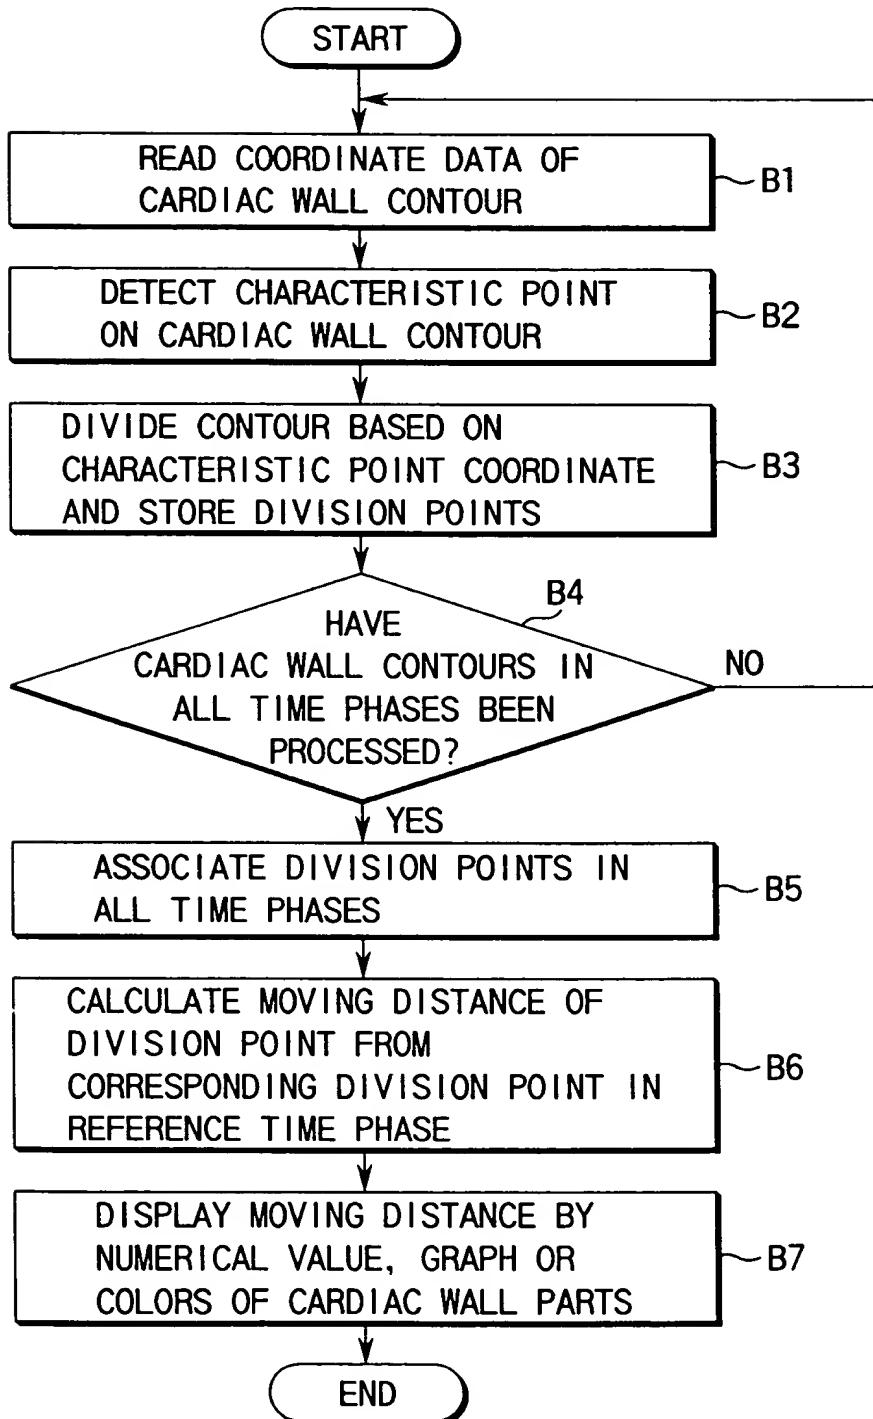


FIG. 61

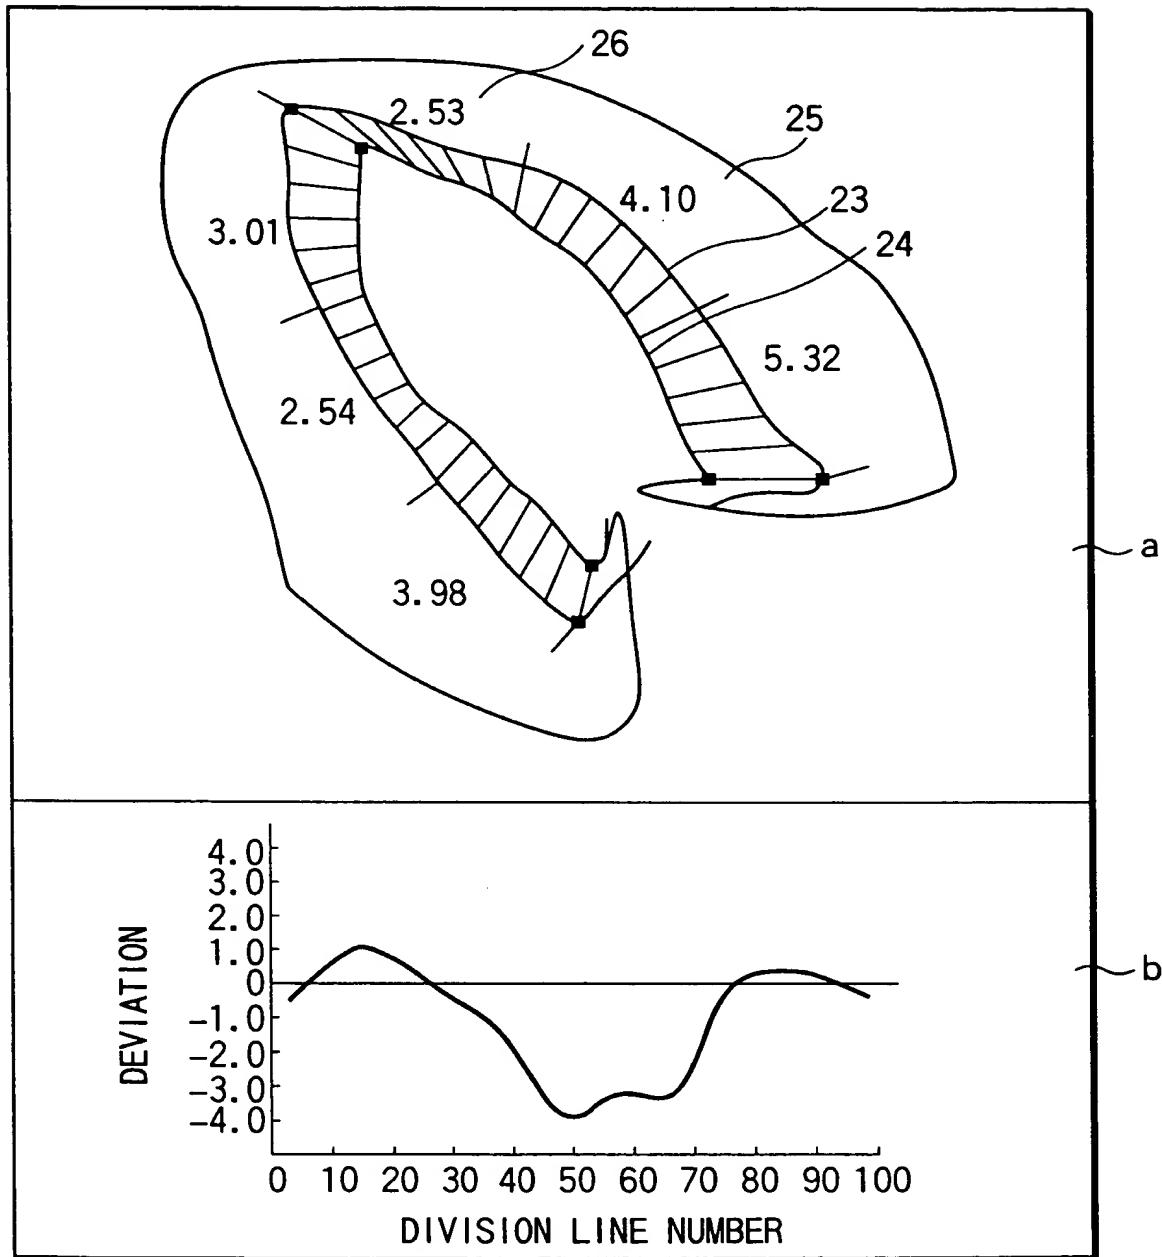


FIG. 62

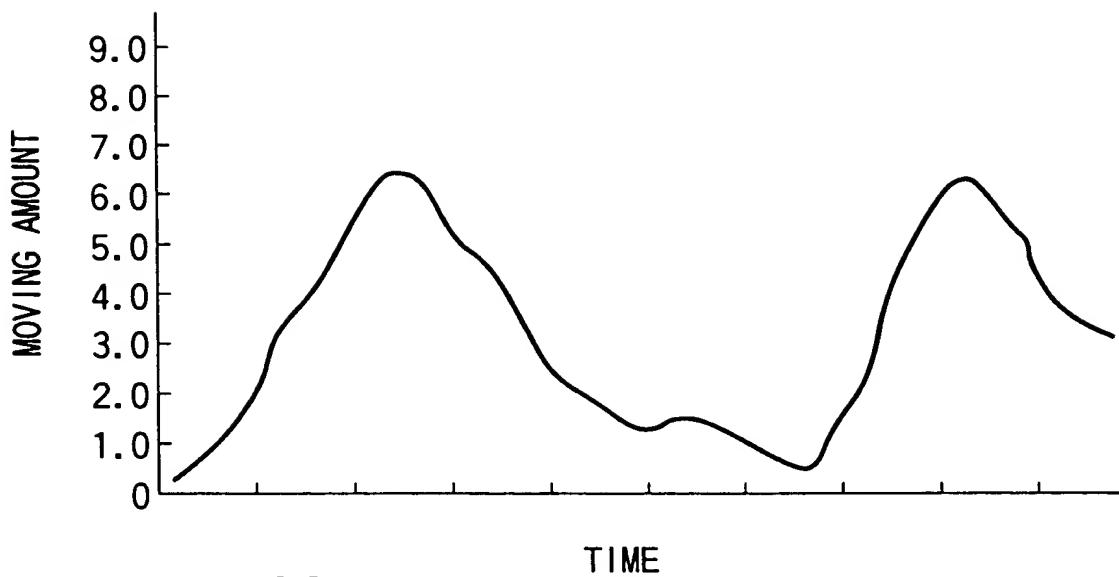


FIG. 63

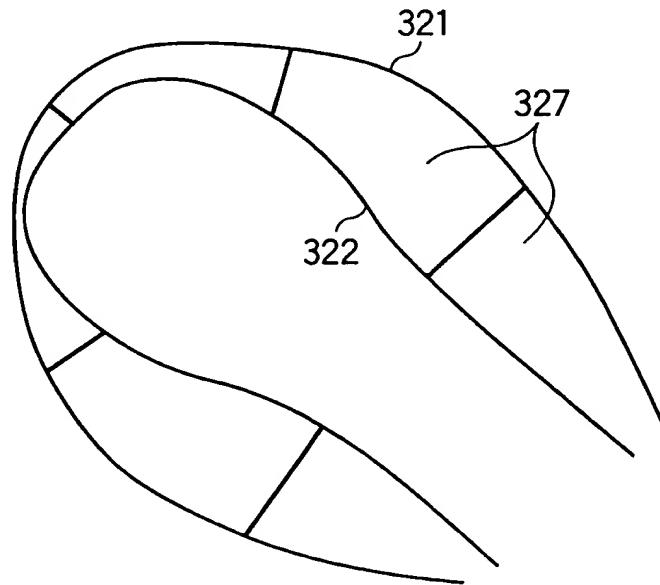


FIG. 64

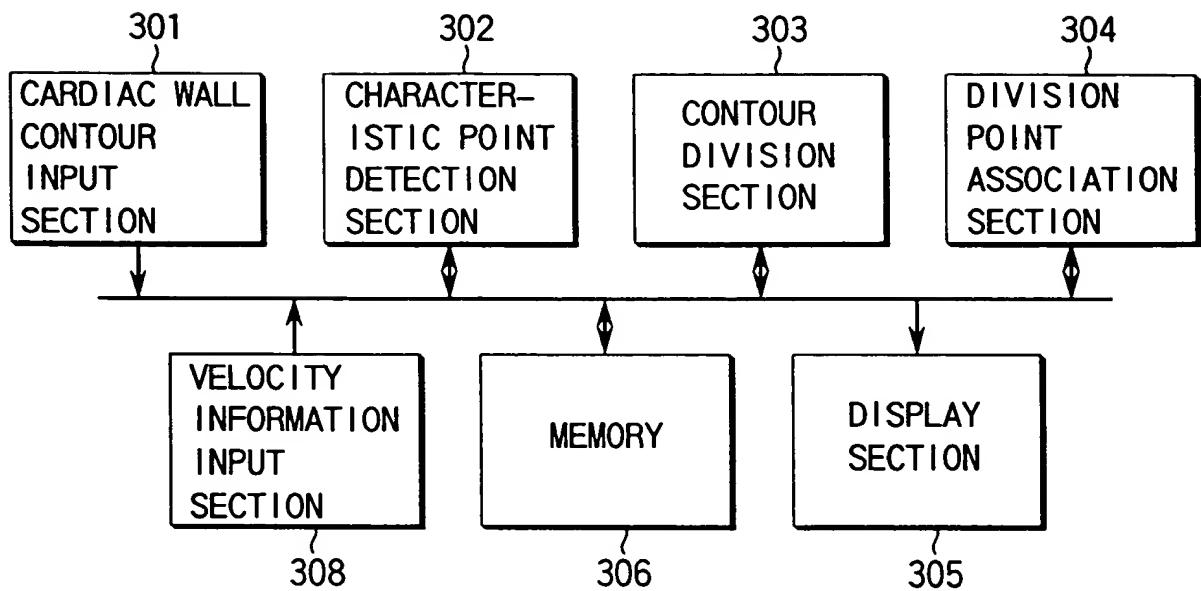


FIG. 65

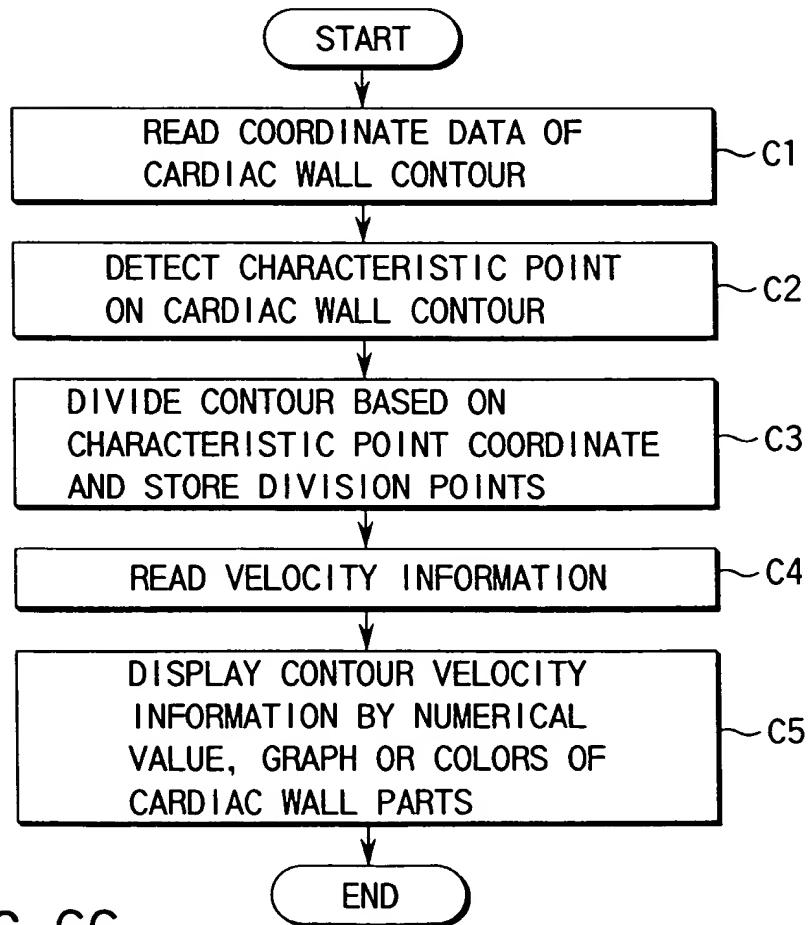


FIG. 66

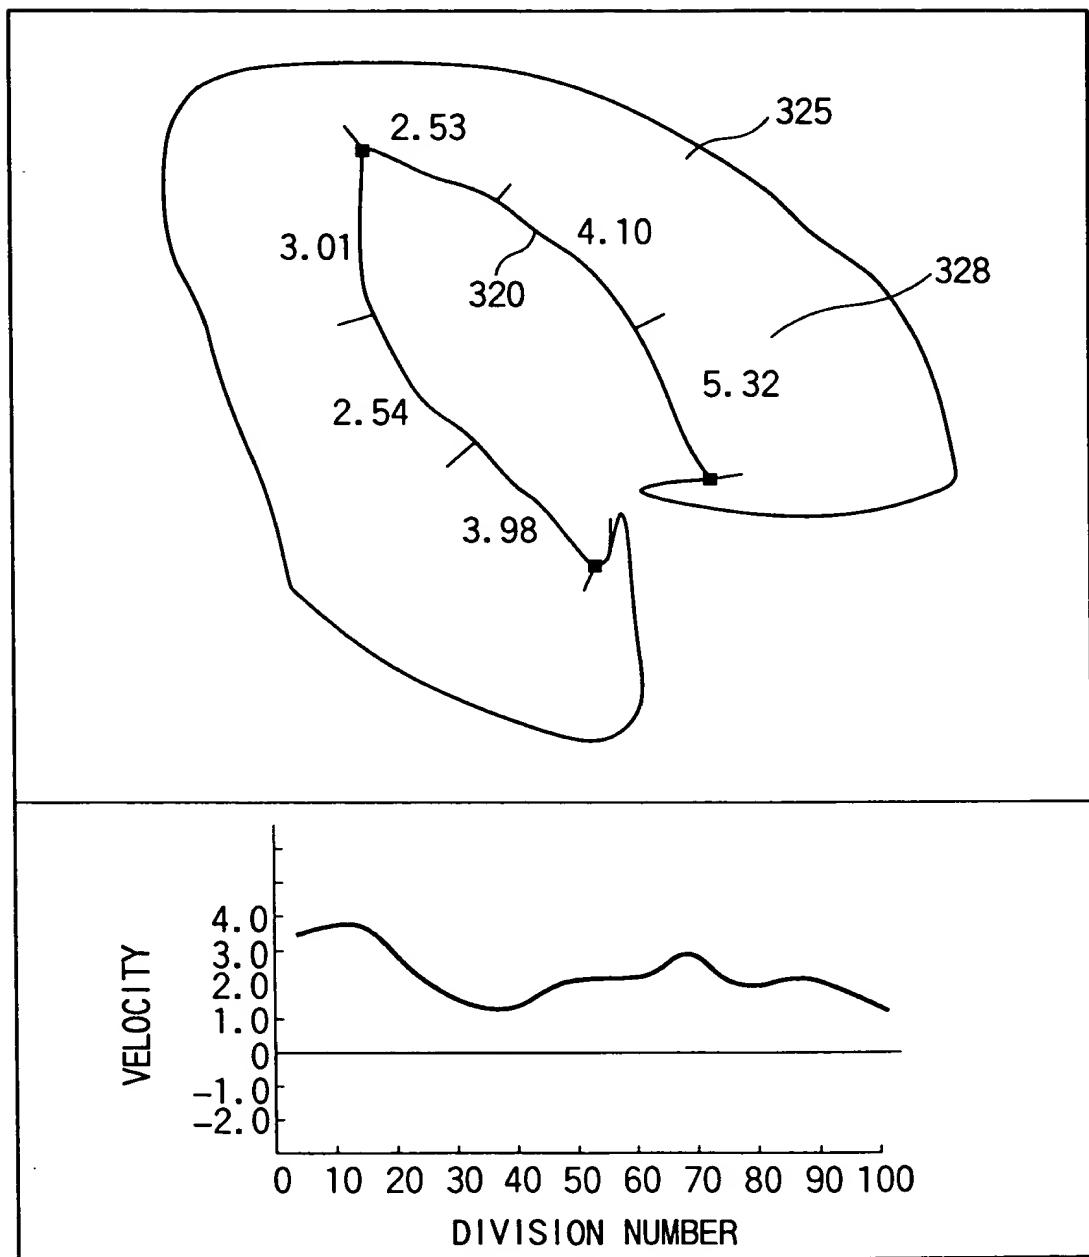


FIG. 67

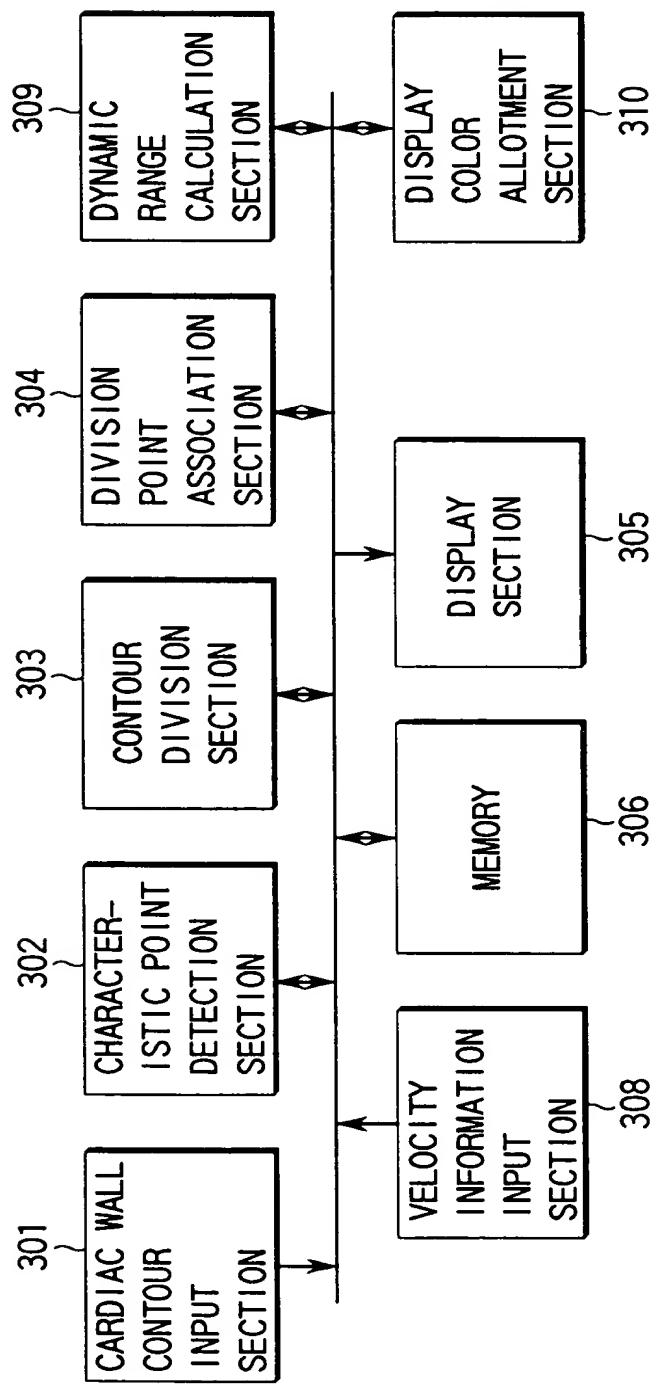


FIG. 68

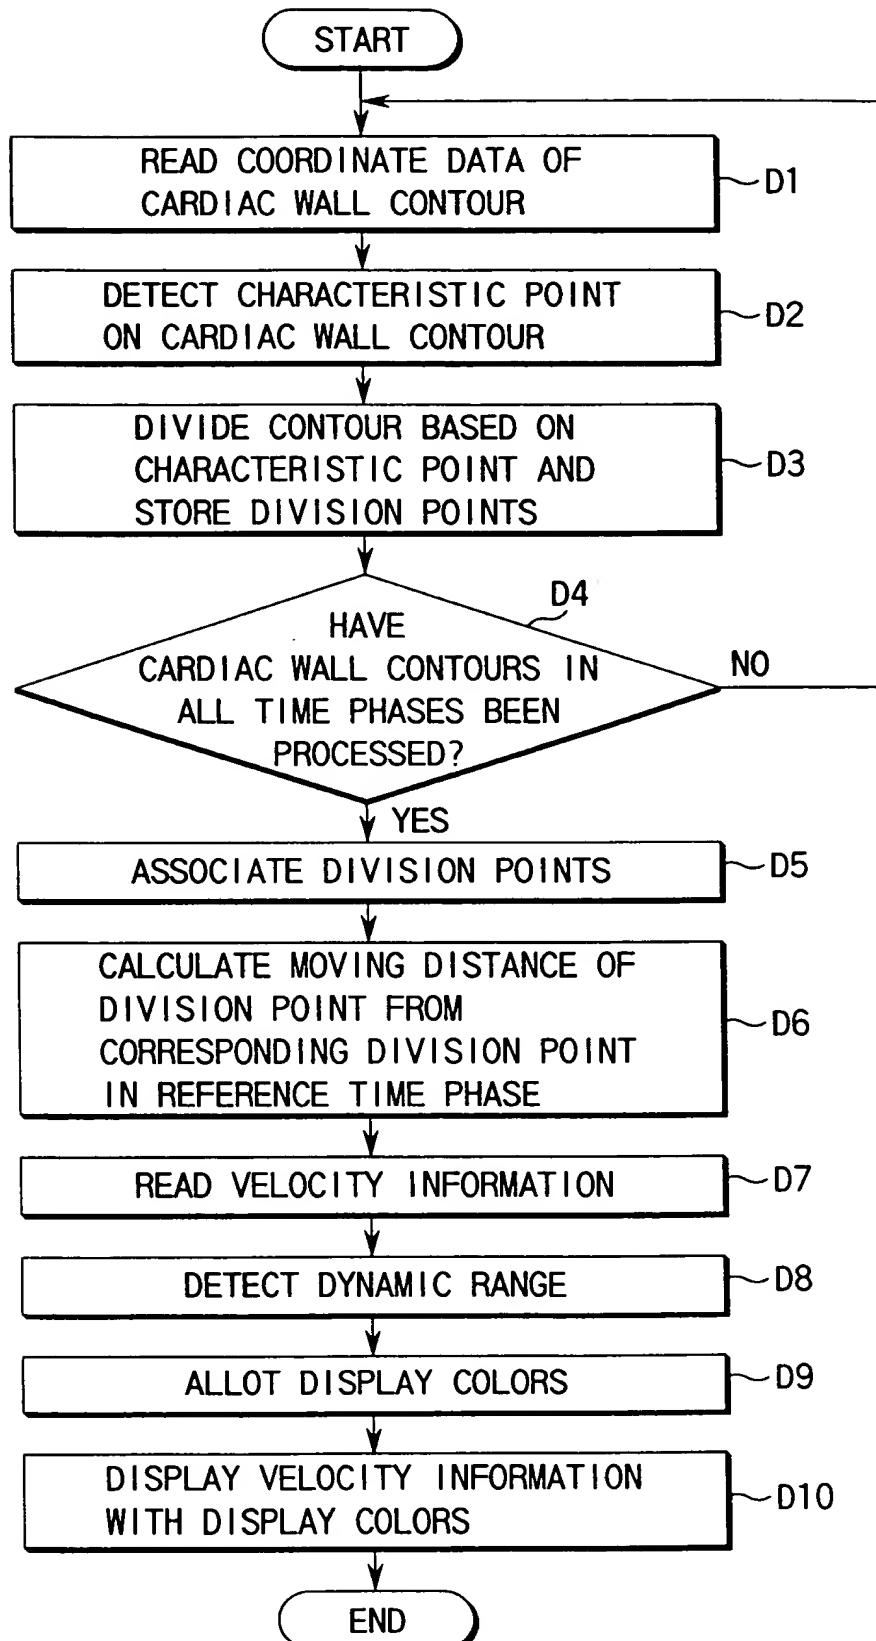


FIG. 69